Immunohematology

ID-System

Product Catalog

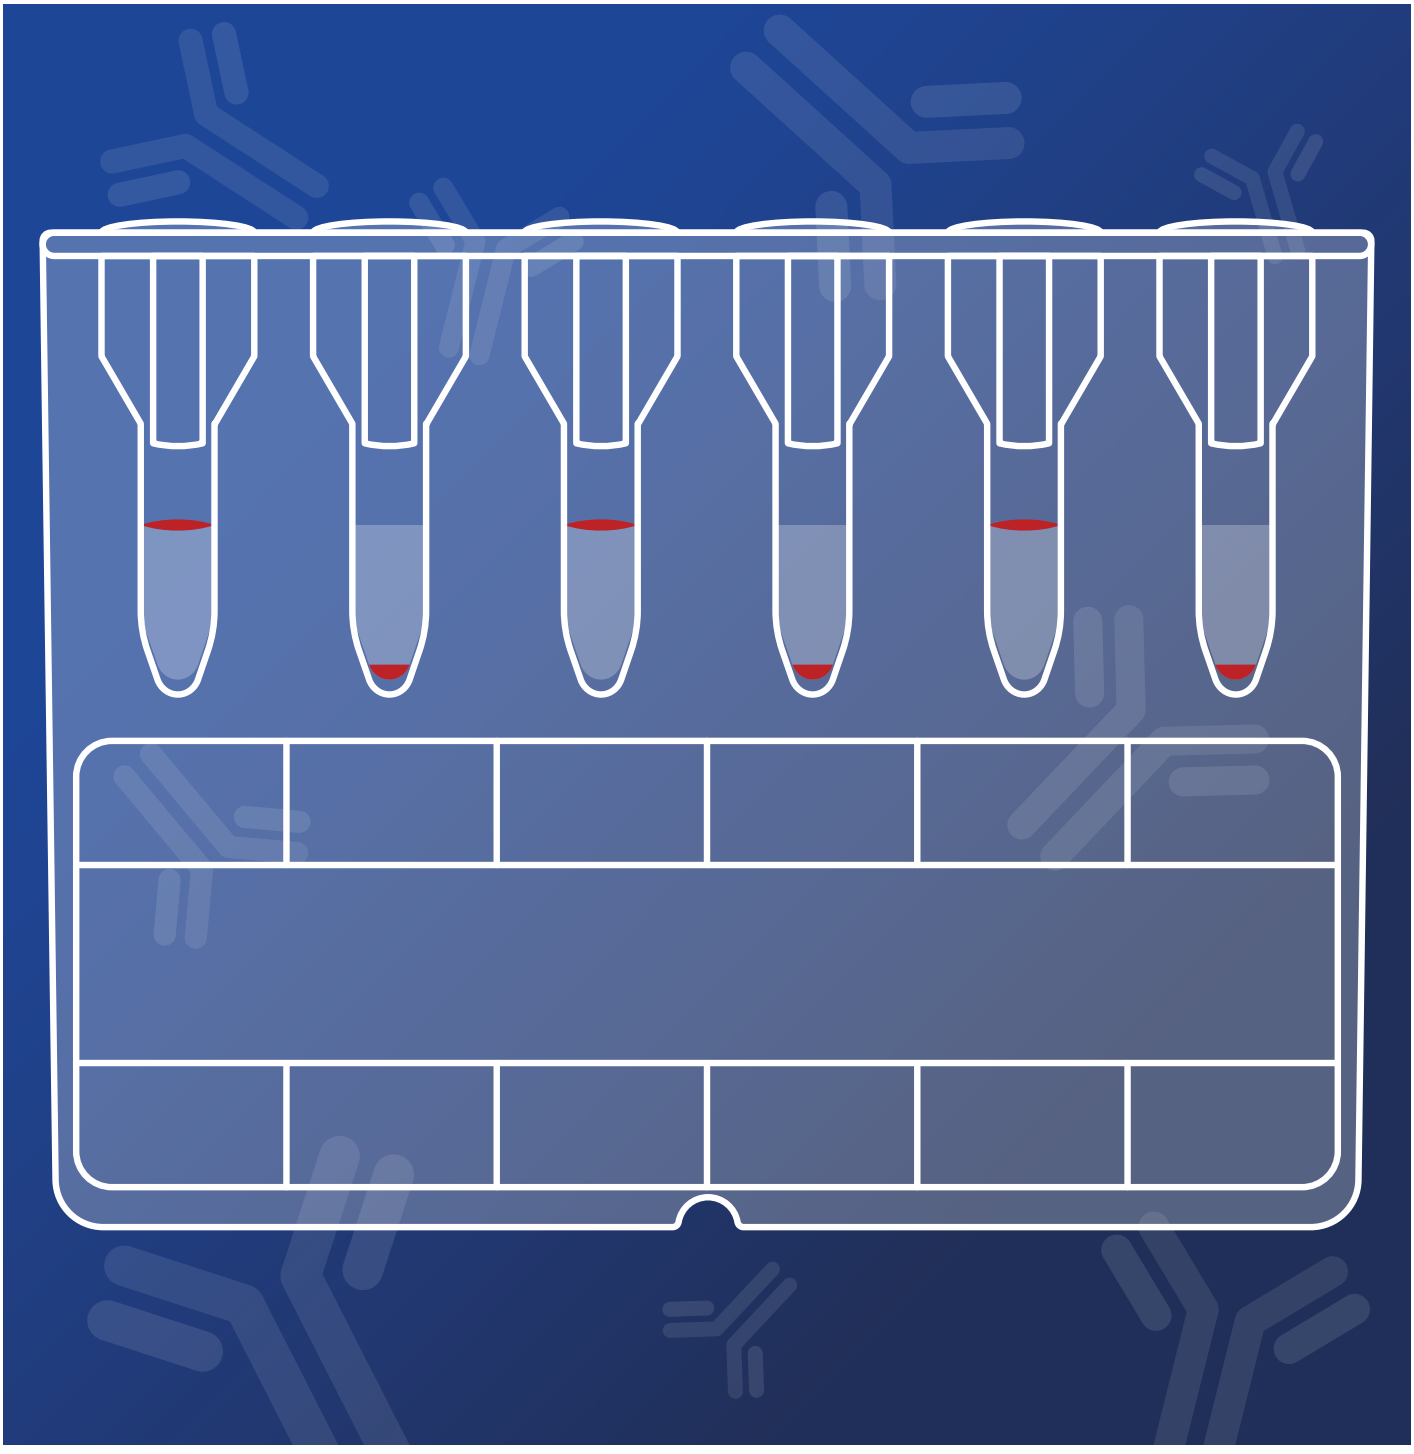

Visit bio-rad.com/diagnostics/immunohematology for more information.

BIO-RAD

Bibliography

[1] Issitt,
P. D. + Anstee: Applied Blood Group Serology, 4th ed. 1998;
Montgomery Scientific Publications,
Miami, Florida, USA.

[2] Mollison P. L.,
Engelfriet C. P. and Contreras
M.: Blood Transfusion in Clinical Medicine. 9th ed. 1993;
Blackwell Scientific Publications, Oxford.

[3] Mollison P. L.,
Engelfriet, C.P. and Contreras,
M.: Blood Transfusion in Clinical Medicine, 10th ed. 1997;
Blackwell Scientific Publications, Oxford.

[4] Daniels G.,
Human Blood Groups
publ.: Blackwell Science Ldt., 1995.

[5] Reid M.E., et al.
The BLOOD GROUP ANTIGEN Facts Book
Elsevier, 3rd Edition, ed. 2012.

BIO-RAD is a trademark of Bio-Rad Laboratories, Inc.
DIACELL, DIAPANEL and IH-500 are trademarks of Bio-Rad Europe, GmbH in certain jurisdictions.

This information is supplied without liability.

Contents

ID-System

Blood Grouping ABO/D with Monoclonal Antibodies	4
Blood Grouping ABO/D with Double Determination of RhD	7
Blood Grouping ABO/D Combined with Reverse Grouping	9
Reverse Grouping	11
Phenotyping Rh/K	12
A Subgroups	14
Typing of Partial RhD	15
Verification of weak D by IAT	16
Antigen Profiles	17
Single Antigen Testing	19
Direct Antiglobulin Test (DAT)	30
Antibody Screening	33
Antibody Identification	35
Compatibility Tests	36
Solutions for Red Blood Cells and Reagents	38
Miscellaneous Solutions	40
Reagent Red Blood Cells for Reverse Grouping	41
Reagent Red Blood Cells for Antibody Screening	42
Reagent Red Blood Cells for Antibody Identification	50
Quality Control for Blood Group Serology	52

It can be that some of the products displayed in this catalog are not available in your country. For further information, please contact your local Bio-Rad contact point.

Frequencies of the different ABO blood groups (according to Reid, M.E. [5]) in the Caucasian population:

O	44%
A	43%
B	9%
AB	4%

Current recommendations for RhD typing suggest that, for transfusion recipients and antenatal patients, anti-D reagents should not detect the DVI phenotype. Individuals possessing the DVI phenotype may produce an anti-D to the missing epitopes after immunization by fetal or transfused RhD positive cells. To ensure that appropriate therapeutic measures are instigated, DVI patient's red cells should be assigned RhD negative status.

Conversely, donor blood should be tested with anti-D that does detect DVI and assigned RhD positive status, to avoid the unit being transfused to an RhD negative or partial D patient.

DiaClon ABO/Rh for Patients

The ID-Card **DiaClon ABO/Rh for Patients** offers a complete test profile for forward grouping of ABO, RhD (DVI neg.) and CDE in one single test profile.

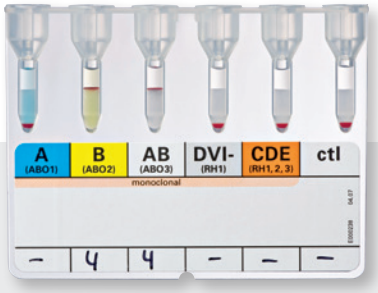

Ordering Information

Catalog #	Description
DiaClon ABO/Rh for Patients	
001044	**A, B, AB, DVI-, CDE, ctl** (Id-n°: 50012) **48 profiles**, 4 x 12
001043	**A, B, AB, DVI-, CDE, ctl** (Id-n°: 50012) **288 profiles**, 24 x 12
001046	**A, B, AB, DVI-, CDE, ctl** (Id-n°: 50012) **720 profiles**, 60 x 12
001045	**A, B, AB, DVI-, CDE, ctl** (Id-n°: 50012) **1,344 profiles**, 112 x 12

Cell lines: **A:** A5, **B:** G1/2, **AB:** ES131 (ES-15), Birma-1, ES-4, **D:** LHM59/20 (LDM3), 175-2, **CDE:** MS-24, MS-26, MS-201, MS-80

DiaClon ABD-Confirmation for Patients

The ABD confirmation ID-Card can be used for the ABO/D blood group control of patients.

Ordering Information

Catalog #	Description
DiaClon ABD-Confirmation for Patients	
001254	**A, B, DVI-, A, B, DVI-** (Id-n°: 50053) **96 profiles**, 4 x 12
001257	**A, B, DVI-, A, B, DVI-** (Id-n°: 50053) **576 profiles**, 24 x 12
001256	**A, B, DVI-, A, B, DVI-** (Id-n°: 50053) **1,440 profiles**, 60 x 12
001255	**A, B, DVI-, A, B, DVI-** (Id-n°: 50053) **2,688 profiles**, 112 x 12

Cell lines: **A:** LM297/628 (LA-2), **B:** LM306/686 (LB-2), **D:** TH28, RUM-1, LDM1

DiaClon ABO/Rh for Newborns DVI+

The ID-Card **DiaClon ABO/Rh for Newborns DVI+** contains monoclonal antibodies.

The anti-D used will not react with all examples of weak D.

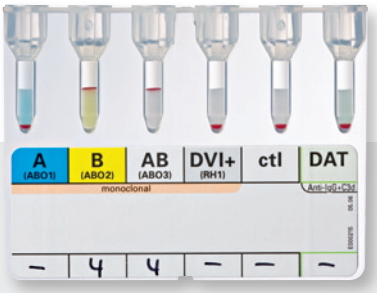

Ordering Information

Catalog #	Description
DiaClon ABO/Rh for Newborns DVI+	
001047	**A, B, AB, DVI+, ctl, DAT** (Id-n°: 50961) **48 profiles**, 4 x 12
001048	**A, B, AB, DVI+, ctl, DAT** (Id-n°: 50961) **288 profiles**, 24 x 12
001049	**A, B, AB, DVI+, ctl, DAT** (Id-n°: 50961) **720 profiles**, 60 x 12
001050	**A, B, AB, DVI+, ctl, DAT** (Id-n°: 50961) **1,344 profiles**, 112 x 12

Cell lines: **A:** LM297/628 (LA-2), **B:** LM306/686 (LB-2), **AB:** ES131 (ES-15), Birma-1, ES-4, **D:** ESD-1M, 175-2

DiaClon ABO/Rh for Newborns DVI-

The monoclonal anti-D used in this ID-Card **DiaClon ABO/Rh for Newborns DVI-** has been selected so as not to react with variant DVI.

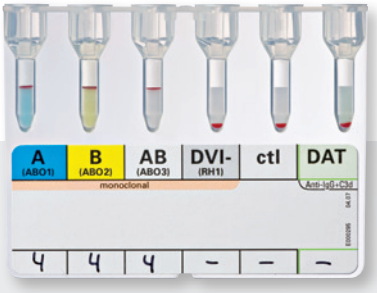

Ordering Information

Catalog #	Description
DiaClon ABO/Rh for Newborns DVI-	
001027	**A, B, AB, DVI-, ctl, DAT** (Id-n°: 50071) **48 profiles**, 4 x 12
001030	**A, B, AB, DVI-, ctl, DAT** (Id-n°: 50071) **288 profiles**, 24 x 12
001028	**A, B, AB, DVI-, ctl, DAT** (Id-n°: 50071) **720 profiles**, 60 x 12
001029	**A, B, AB, DVI-, ctl, DAT** (Id-n°: 50071) **1,344 profiles**, 112 x 12

Cell lines: **A:** LM297/628 (LA-2), **B:** LM306/686 (LB-2), **AB:** ES131 (ES-15), Birma-1, ES-4, **D:** LDM3, 175-2

DiaClon ABO/Rh for Donors

This ID-Card for donors offers a complete test profile for forward grouping of ABO, RhD and CDE in one single test procedure.

The monoclonal anti-D used has been selected so as to react with variant DVI.

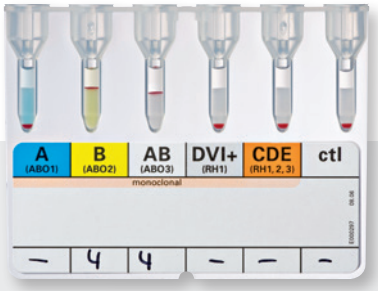

Ordering Information

Catalog #	Description
DiaClon ABO/Rh for Donors	
001037	**A, B, AB, DVI+, CDE, ctl** (Id-n°: 51011) **48 profiles**, 4 x 12
001033	**A, B, AB, DVI+, CDE, ctl** (Id-n°: 51011) **288 profiles**, 24 x 12
001039	**A, B, AB, DVI+, CDE, ctl** (Id-n°: 51011) **720 profiles**, 60 x 12
001038	**A, B, AB, DVI+, CDE, ctl** (Id-n°: 51011) **1,344 profiles**, 112 x 12

Cell lines: **A:** A5, **B:** G1/2, **AB:** ES131 (ES-15), Birma-1, ES-4, **D:** ESD-1M, 175-2, **CDE:** MS-24, MS-26, MS-201, MS-80

DiaClon ABD-Confirmation for Donors

For the ABO/D blood group control of donors.

Ordering Information

Catalog #	Description
DiaClon ABD-Confirmation for Donors	
001134	**A, B, DVI+/A, B, DVI+** (Id-n°: 51051) **96 profiles**, 4 x 12
001133	**A, B, DVI+/A, B, DVI+** (Id-n°: 51051) **576 profiles**, 24 x 12
001136	**A, B, DVI+/A, B, DVI+** (Id-n°: 51051) **1,440 profiles**, 60 x 12
001135	**A, B, DVI+/A, B, DVI+** (Id-n°: 51051) **2,688 profiles**, 112 x 12

Cell lines: **A:** LM297/628 (LA-2), **B:** LM306/686 (LB-2), **D:** ESD-1M, 175-2

DiaClon ABO/D

The first anti-D detects the presence of the variant DVI, the second anti-D is negative for the variant DVI. All antibodies in this ID-Card are monoclonal.

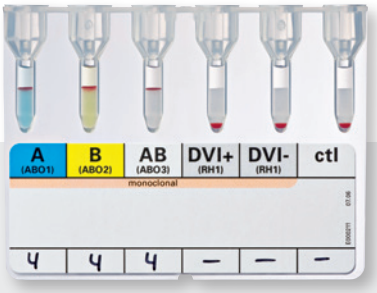

Ordering Information

Catalog #	Description
DiaClon ABO/D	
001324	**A, B, AB, DVI+, DVI-, ctl** (Id-n°: 50481) **48 profiles**, 4 x 12
001323	**A, B, AB, DVI+, DVI-, ctl** (Id-n°: 50481) **288 profiles**, 24 x 12
001326	**A, B, AB, DVI+, DVI-, ctl** (Id-n°: 50481) **720 profiles**, 60 x 12
001325	**A, B, AB, DVI+, DVI-, ctl** (Id-n°: 50481) **1,344 profiles**, 112 x 12

Cell lines: **A:** A5, **B:** G1/2, **AB:** ES131 (ES-15), Birma-1, ES-4, **D:** ESD-1M, 175-2, **D:** LHM59/20 (LDM3), 175-2

DiaClon ABO/D + DAT

With this ID-Card a complete profile for ABO forward grouping and RhD status can be obtained in one single procedure, including a Direct Antiglobulin Test (DAT).

The two anti-D antibodies in the ID-Card are negative for the variant DVI.

The test procedure is thus suitable for patients and not recommended for donors.

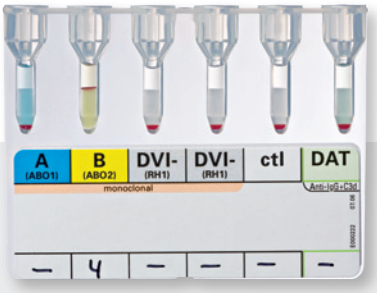

Ordering Information

Catalog #	Description
DiaClon ABO/D + DAT	
001344	**A, B, DVI-, DVI-, ctl, DAT** (Id-n°: 50492) **48 profiles**, 4 x 12
001347	**A, B, DVI-, DVI-, ctl, DAT** (Id-n°: 50492) **288 profiles**, 24 x 12
001346	**A, B, DVI-, DVI-, ctl, DAT** (Id-n°: 50492) **720 profiles**, 60 x 12
001345	**A, B, DVI-, DVI-, ctl, DAT** (Id-n°: 50492) **1,344 profiles**, 112 x 12

Cell lines: **A:** A5, **B:** G1/2, **D:** LHM50/3 (LDM1), TH-28, RUM-1, **D:** LHM59/20 (LDM3), 175-2

DiaClon ABO/DVI- for Patients

Testing protocols for both patients and newborns

This ID-Card is used for ABO forward grouping and double RhD determination for patients as well as for newborns.

Please note that certain guidelines require the detection of DVI for newborns.

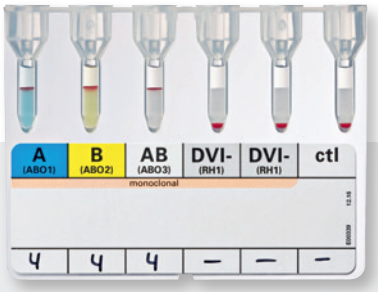

Ordering Information

Catalog #	Description
DiaClon ABO/DVI- for Patients	
001294	**A, B, AB, DVI-, DVI-, ctl** (Id-n°: 52040) **48 profiles**, 4 x 12
001297	**A, B, AB, DVI-, DVI-, ctl** (Id-n°: 52040) **288 profiles**, 24 x 12
001296	**A, B, AB, DVI-, DVI-, ctl** (Id-n°: 52040) **720 profiles**, 60 x 12

Cell lines: **A:** LM297/628 (LA-2), **B:** LM306/686 (LB-2), **AB:** ES131 (ES-15), Birma-1, ES-4, **D:** LHM50/3 (LDM1), TH-28, RUM-1, **D:** LHM59/20 (LDM3), 175-2

DiaClon ABO/DVI-

Testing protocols for both patients and newborns

This ID-Card is used for ABO forward grouping and double RhD determination for patients as well as for newborns.

Please note that certain guidelines require the detection of DVI for newborns.

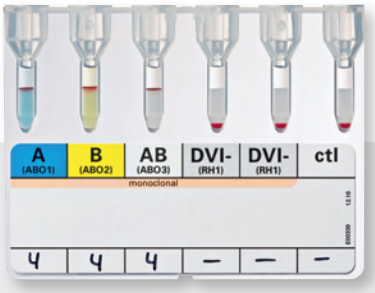

Ordering Information

Catalog #	Description
DiaClon ABO/DVI-	
001424	**A, B, AB, DVI-, DVI-, ctl** (Id-n°: 52050) **48 profiles**, 4 x 12
001427	**A, B, AB, DVI-, DVI-, ctl** (Id-n°: 52050) **288 profiles**, 24 x 12
001425	**A, B, AB, DVI-, DVI-, ctl** (Id-n°: 52050) **1,344 profiles**, 112 x 12

Cell lines: **A:** A5, **B**: G1/2, **AB:** ES131 (ES-15), Birma-1, ES-4, **D:** LHM50/3 (LDM1), TH-28, RUM-1, **D:** LHM59/20 (LDM3), 175-2

DiaClon ABO/DVI+/DVI- + DAT

With the ID-Card **DiaClon ABO/DVI+/DVI- + DAT** a complete profile for ABO forward grouping and RhD status can be obtained in one single test procedure, including a Direct Antiglobulin Test (DAT).

The first anti-D detects the presence of the variant DVI, the second anti-D is negative for the variant DVI.

The test procedure may therefore be used for both patients and donors.

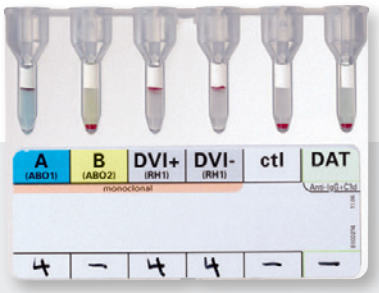

Ordering Information

Catalog #	Description
DiaClon ABO/DVI+/DVI- + DAT	
001374	**A, B, DVI+, DVI-, ctl, DAT** (Id-n°: 51160) **48 profiles**, 4 x 12
001376	**A, B, DVI+, DVI-, ctl, DAT** (Id-n°: 51160) **720 profiles**, 60 x 12

Cell lines: **A:** A5, **B:** G1/2, **D:** ESD-1M, 175-2, **D:** LHM59/20 (LDM3, 175-2)

DiaClon ABO/D + Reverse Grouping

The microtube ctl is the negative control. Two microtubes with neutral gel serve for reverse grouping with A_1 and B cells.

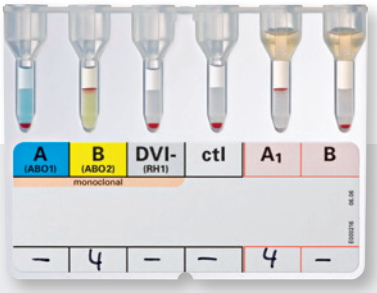

Ordering Information

Catalog #	Description
DiaClon ABO/D + Reverse Grouping	
001234	**A, B, DVI-, ctl/A_1, B** (Id-n°: 50092) **48 profiles**, 4 x 12
001237	**A, B, DVI-, ctl/A_1, B** (Id-n°: 50092) **288 profiles**, 24 x 12
001236	**A, B, DVI-, ctl/A_1, B** (Id-n°: 50092) **720 profiles**, 60 x 12
001235	**A, B, DVI-, ctl/A_1, B** (Id-n°: 50092) **1,344 profiles**, 112 x 12

Cell lines: **A:** A5, **B:** G1/2, **D:** LHM59/20 (LDM3), 175-2

DiaClon ABO/D + Reverse Grouping

The ID-Card **DiaClon ABO/D + Reverse Grouping** allows combined testing of forward and reverse grouping as well as a double RhD determination with two anti-D selected to not detecting the variant DVI.

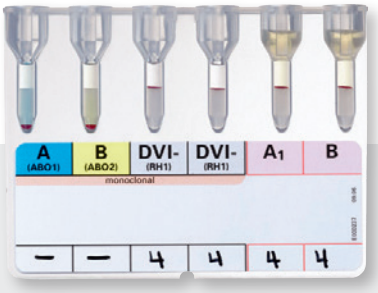

Ordering Information

Catalog #	Description
DiaClon ABO/D + Reverse Grouping	
001248	**A, B, DVI-, DVI-, A_1, B** (Id-n°: 50742) **720 profiles**, 60 x 12
001249	**A, B, DVI-, DVI-, A_1, B** (Id-n°: 50742) **1,344 profiles**, 112 x 12

Cell lines: **A:** A5, **B:** LB-2, **D:** LHM 50/3 (LDM1), TH-28, RUM-1, **D:** LHM 59/20 (LDM3), 175-2

DiaClon ABO/D (DVI+, DVI-) + Reverse Grouping

The ID-Card **DiaClon ABO/D (DVI+, DVI-) + Reverse Grouping** allows combined testing of forward and reverse grouping as well as a double RhD determination.

The first anti-D is selected for detecting the variant DVI, the second anti-D is selected to be negative for the variant DVI.

The test procedure may therefore be used for both patients and donors.

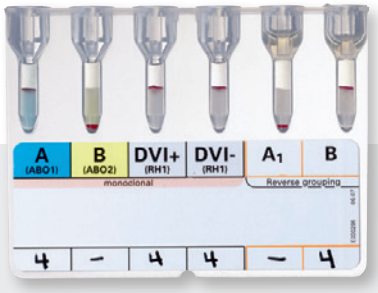

Ordering Information

Catalog #	Description
DiaClon ABO/D (DVI+, DVI-) + Reverse Grouping	
001386	**A, B, DVI+, DVI-, A_1, B** (Id-n°: 50981) **720 profiles**, 60 x12

Cell lines: **A:** A5, **B:** G1/2, **D:** ESD-1M, 175-2, **D:** LHM 50/3 (LDM1), TH-28, RUM-1

DiaClon ABO/D + Reverse Grouping for Donors

The ID-Card **DiaClon ABO/D + Reverse Grouping for Donors** allows combined testing of forward and reverse grouping as well as RhD determination for confirmation of previously fully tested samples with established blood group status.

The monoclonal anti-D used has been selected so as to react with variant DVI.

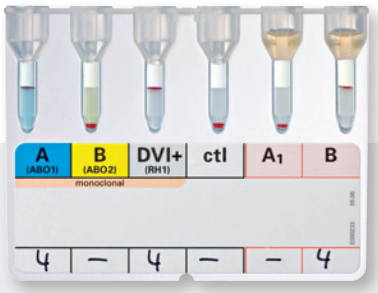

Ordering Information

Catalog #	Description
DiaClon ABO/D + Reverse Grouping for Donors	
12010791	**A, B, DVI+, ctl/A_1, B** (Id-n°: 51090) **48 profiles**, 4 x 12
001365	**A, B, DVI+, ctl/A_1, B** (Id-n°: 51090) **1,344 profiles**, 112 x 12

Cell lines: **A:** A5, **B:** G1/2, **D:** ESD-1M, 175-2

NaCl, Enzyme Test and Cold Agglutinins

The **ID-Card NaCl, Enzyme Test and Cold Agglutinins** is suitable for reverse grouping in any combination with **ID-DiaCell ABO** Reagent Red Blood Cells and any ABO ID-Card for forward grouping for manual use as well as on instruments.

Ordering Information

Catalog #	Description
NaCl, Enzyme Test and Cold Agglutinins	
005014	**6 x tests** (Id-n°: 50520) **288 profiles**, 4 x 12
005017	**6 x tests** (Id-n°: 50520) **1,728 profiles,** 24 x 12
005016	**6 x tests** (Id-n°: 50520) **4,320 profiles**, 60 x 12
005015	**6 x tests** (Id-n°: 50520) **8,064 profiles**, 112 x 12

Besides the RhD antigen, other important antigens of the Rh Blood Group System are: C, E, c and e. According to Reid, M.E. [5], their frequencies in the Caucasian population are as follows:

C	68%
c	80%
E	29%
e	98%
D	85%

Approximately 9% of the Caucasian population are K positive. The K antigen is strongly immunogenic. Anti-K has been reported as the cause of hemolytic transfusion reactions, both immediate and delayed, and hemolytic disease of the newborn.

DiaClon Rh-Subgroups + K

This ID-Card offers a complete profile of the Rh phenotype including K-typing.

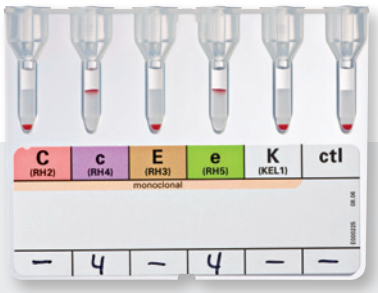

Ordering Information

Catalog #	Description
DiaClon Rh-Subgroups + K	
002124	**C, c, E, e, K, ctl** (Id-n°: 50110) **48 profiles**, 4 x 12
002127	**C, c, E, e, K, ctl** (Id-n°: 50110) **288 profiles**, 24 x 12
002126	**C, c, E, e, K, ctl** (Id-n°: 50110) **720 profiles**, 60 x 12
002125	**C, c, E, e, K, ctl** (Id-n°: 50110) **1,344 profiles**, 112 x 12

Cell lines: **C:** MS-24, **c:** MS-33, **E:** MS-260, **e:** MS-16, MS-21, MS-63, **K:** MS-56

DiaClon Rh + K Pheno II

This ID-Card offers a complete profile of the Rh phenotype including K-typing.

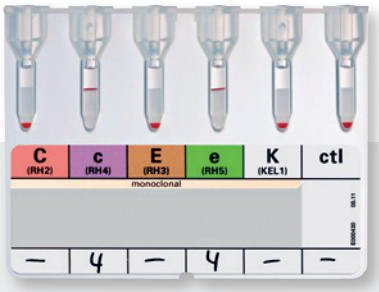

Ordering Information

Catalog #	Description
DiaClon Rh + K Pheno II	
002224	**C, c, E, e, K, ctl** (Id-n°: 50710) **48 profiles**, 4 x 12
002227	**C, c, E, e, K, ctl** (Id-n°: 50710) **288 profiles**, 24 x 12
002226	**C, c, E, e, K, ctl** (Id-n°: 50710) **720 profiles**, 60 x 12
002225	**C, c, E, e, K, ctl** (Id-n°: 50710) **1,344 profiles**, 112 x 12

Cell lines: **C:** MS-273, P3x25513G8, **c:** 951, **E:** MS-80, MS-258, **e:** MS-62, P3GD512, **K:** AEK4

DiaClon Rh-Subgroups + C^w + K

The ID-Card **DiaClon Rh-Subgroups + C^w + K** is designed for the determination of the presence or absence of the C (RH2), C^w (RH8), c (RH4), E (RH3), e (RH5) and K (KEL1) antigens on human Red Blood Cells, for manual use as well as on instruments.

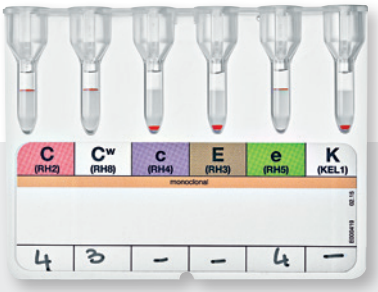

Ordering Information

Catalog #	Description
DiaClon Rh-Subgroups + C^w + K	
002134	**C, C^w, c, E, e, K** (Id-n°: 52000) **48 profiles**, 4 x 12
002137	**C, C^w, c, E, e, K** (Id-n°: 52000) **288 profiles**, 24 x 12
002136	**C, C^w, c, E, e, K** (Id-n°: 52000) **720 profiles**, 60 x 12
002135	**C, C^w, c, E, e, K** (Id-n°: 52000) **1,344 profiles**, 112 x 12

Cell lines: **C:** MS-273, P3x25513G8, **C^w:** MS-110, **c:** 951, **E:** MS-80, MS-258, **e:** MS-62, P3GD512, **K:** AEK4

Control Card A

The ID-Card **Control Card A** is designed to validate the reactions obtained with the ID-Cards **DiaClon Rh-Subgroups** + **C^w** + **K** and **DiaClon Anti-C^w**.

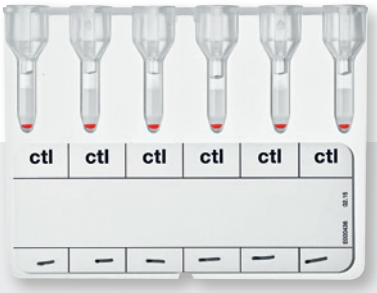

Ordering Information

Catalog #	Description
Control Card A	
001711	**6 x ctl** (Id-n°: 52020) **72 tests**, 1 x 12
001714	**6 x ctl** (Id-n°: 52020) **288 tests**, 4 x 12

DiaClon RhD + Phenotype

This ID-Card offers a complete profile of the Rh phenotype and the monoclonal anti-D reagent has been selected so as not to react with variants DVI.

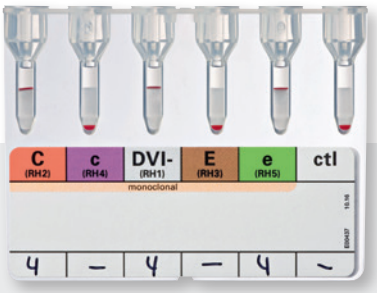

Ordering Information

Catalog #	Description
DiaClon RhD + Phenotype	
002234	**C, c, DVI-, E, e, ctl** (Id-n°: 52030) **48 profiles**, 4 x 12
002237	**C, c, DVI-, E, e, ctl** (Id-n°: 52030) **288 profiles**, 24 x 12

The reagent **Anti-A_1 Absorbed** agglutinates A_1 cells but reacts negatively or only weakly with A_2 cells.

Approximately 80% of group A or AB individuals have Red Blood Cells that are agglutinated by anti-A1 and are thus classified as A_1 or A_1B.

Anti-A_1 Absorbed

ID-Card with 6 microtubes containing anti-A1, human, within the gel matrix.

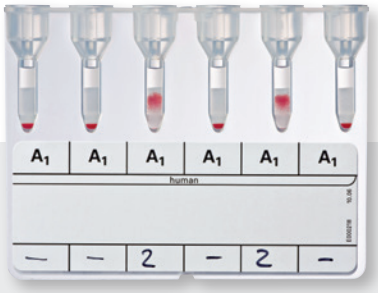

Ordering Information

Catalog #	Description
Anti-A_1 Absorbed	
001811	**6 x A_1** (Id-n°: 50140) human **72 tests**, 1 x 12

The H antigen is present on all human Red Blood Cells, except those with the phenotype O^h (Bombay blood group). H is the precursor substance for A and B antigens.

For the classification of A subgroup status, anti-H should be used in conjunction with anti-A, anti-AB and anti-A1.

DiaClon Anti-H

ID-Card with 6 microtubes containing anti-H, monoclonal, within the gel matrix.

Ordering Information

Catalog #	Description
DiaClon Anti-H	
001911	**6 x H** (Id-n°: 50150) **72 tests**, 1 x 12

Cell lines: H-86-50+H89/8

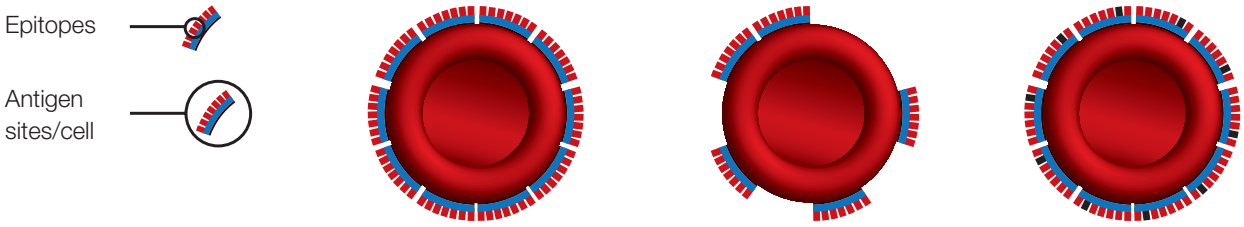

	Normal D-Antigen	Weak D	Partial D
Epitopes:	Normal	Normal	Reduced (Lacking)
Antigen sites/cell:	Normal	Reduced	Normal or reduced

ID-Partial RhD Typing Set

For the Typing of Partial RhD

The **ID-Partial RhD Typing Set** consists of 6 monoclonal anti-D reagents that help further characterize the RhD antigen after routine RhD typing. The kit also contains 12 ID-Cards.

The reagents help with the differentiation of categories DII, DIV, DV, DVI, DVII, DFR, DBT and R_0^{Har}.

Ordering Information

Catalog #	Description
ID-Partial RhD Typing Set	
001451	**Test Kit ID-Partial RhD Typing Set** (Id-n°: 46170), **12 tests** **ID-Cards,** 1 x 12 **ID-Anti-D 1-6**, 6 x 0.4 ml

Cell lines: LHM76/55, LHM77/64, LHM70/45, LHM59/19, LHM169/80, LDM1

Interpretation Table

Cell line	Anti-D	DII	DIII	DIVa	DIVb	DV	DVI	DVII	DFR	DBT	DHAR
LHM76/55 (IgG)	1	+	+	-	-	+	+	+	+	-	-
LHM77/64 (IgG)	2	-	+	-	-	+	+	+	+	-	-
LHM70/45 (IgG)	3	+	+	-	-	-	-	+	-	-	-
LHM59/19 (IgG)	4	+	+	+	+	+	-	+ -*	-	+	-
LHM169/80 (IgG)	5	+	+	+	+	+	-	+	+	-	-
LDM1 (IgM)	6	+	+	+	+	+ -	-	+	-	+	+ -

** A weaker reaction can be observed with this antibody, in comparison with the other 5 sera.*

ID-DiaClon Anti-D

For the confirmation of weak D by IAT

The increasing use of monoclonal anti-D from different cell lines can create problems in the interpretation of D antigen testing, in particular the differentiation of weak D and partial D.

ID-DiaClon Anti-D for confirmation of weak D by IAT containing monoclonal IgG anti-D supplied as a ready-to-use reagent in vials of 5 ml.

Ordering Information

Catalog #	Description
ID-DiaClon Anti-D	
007531	(Id-n°: 09410) ESD1 **100 tests**, 1 x 5 ml

Coombs Anti-IgG

ID-Card **Coombs Anti-IgG** with 6 microtubes containing anti-human globulin anti-IgG (rabbit), within the gel matrix.

Ordering Information

Catalog #	Description
Coombs Anti-IgG	
004024	**6 x AHG (Anti-IgG)** (Id-n°: 50540) rabbit **288 tests**, 4 x 12
004027	**6 x AHG (Anti-IgG)** (Id-n°: 50540) rabbit **1,728 tests**, 24 x 12
004026	**6 x AHG (Anti-IgG)** (Id-n°: 50540) rabbit **4,320 tests**, 60 x 12
004025	**6 x AHG (Anti-IgG)** (Id-n°: 50540) rabbit **8,064 tests**, 112 x 12

LISS/Coombs

Ordering Information

Catalog #	Description
LISS/Coombs	
004014	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **288 profiles**, 4 x 12
004017	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **1,728 profiles**, 24 x 12
004016	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **4,320 profiles**, 60 x 12
004015	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **8,064 profiles**, 112 x 12

C3d: cell line C139-9

ABO and RhD compatible blood is used for transfusion. In certain cases, Rh phenotypes and the status of the Kell (KEL) Blood Group System are also taken into account.

Antigens from other Blood Group Systems are generally not considered. However, when a clinically significant antibody is present, appropriate antigen negative blood should be used. For such cases, the rapid availability of fully typed donor blood is of great advantage. The ID-System facilitates complete antigen profiling.

ID-Antigen Profile I

In the ID-Card **ID-Antigen Profile I**, the gel suspensions contain the corresponding antibodies, requiring only the addition of the Red Blood Cell suspension (in **ID-Diluent 1**).

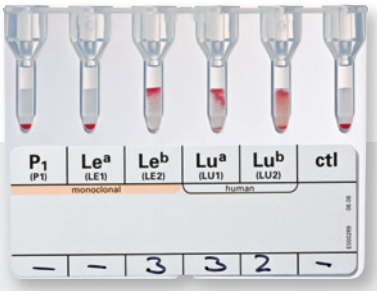

Ordering Information

Catalog #	Description
ID-Antigen Profile I	
008510	**P_1, Le^a, Le^b, Lu^a, Lu^b, ctl** (Id-n°: 50372) **12 profiles**, 1 x 12

Cell lines: **P_1:** 650, **Le^a:** P3N20V3 + LM112/161, **Le^b:** LM129/181
Lu^a/Lu^b human antibodies

ID-Antigen Profile II

In the ID-Card **ID-Antigen Profile II**, the gel suspensions contain the corresponding antibodies, requiring only the addition of the Red Blood Cell suspension (in **ID-Diluent 1**).

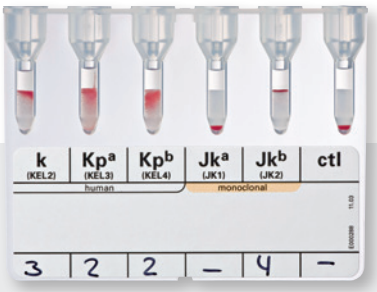

Ordering Information

Catalog #	Description
ID-Antigen Profile II	
008610	**k, Kp^a, Kp^b, Jk^a, Jk^b, ctl** (Id-n°: 50380) **12 profiles**, 1 x 12

Cell lines: **Jk^a:** MS-15, **Jk^b:** MS-8
k/Kp^a/Kp^b human antibodies

ID-Antigen Profile III

In the ID-Card **ID-Antigen Profile III**, the first 2 microtubes contain neutral gel and the last 4, gel with polyspecific anti-human globulin (AHG): the corresponding antibodies (ID-test sera, specially adapted for the ID-System) are added after the Red Blood Cell suspension (in **ID-Diluent 2**).

Ordering Information

Catalog #	Description
ID-Antigen Profile III	
008701	**ID-Card: M, N, S, s, Fy^a, Fy^b** (Id-n°: 50390) **12 profiles**, 1 x 12
008712	**Test sera ID-M, N, S, s, Fy^a, Fy^b** (Id-n°: 45460) **90 profiles**, 6 x 5 ml

M/N monoclonal antibodies
Cell lines: **M:** LM110/140 (LM-1), **N:** 1422 C7
S/s/Fy^a/Fy^b human antibodies

DiaClon Anti-C^w

The ID-Card **DiaClon Anti-C^w** is designed for the determination of the presence or absence of the C^w antigen (RH8) on human Red Blood Cells, for manual use as well as on instruments.

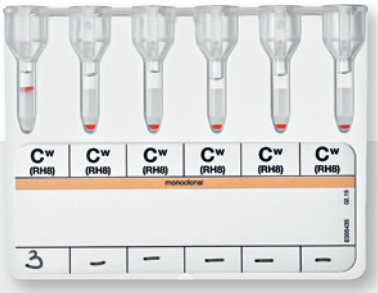

Ordering Information

Catalog #	Description
DiaClon Anti-C^w	
001321	**6 x C^w** (Id-n°: 52010) **72 tests**, 1 x 12

Cell line: MS-110

Control Card A

The ID-Card **Control Card A** is designed to validate the reactions obtained with the ID-Cards **DiaClon Anti-C^w** and **DiaClon Rh-Subgroups** + **C^w** + **K**.

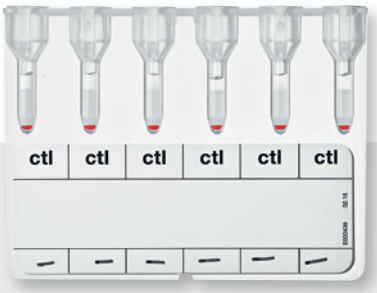

Ordering Information

Catalog #	Description
Control Card A	
001711	**6 x ctl** (Id-n°: 52020) **72 tests**, 1 x 12
001714	**6 x ctl** (Id-n°: 52020) **288 tests**, 4 x 12

The Kell (KEL) Blood Group System (ISBT, number 006) is currently known to contain 35 antigens, numbered K1 to K38 (K8, K9 and K15 are now obsolete). According to Reid, M.E. [5], the phenotype frequencies of the antithetical antigens K (KEL1) and k (KEL2) in the Caucasian population are as follows:

KK	0.2%
Kk	8.8%
kk	91%

The antibodies of the Kell (KEL) Blood Group System have been associated with transfusion reactions and hemolytic disease of the newborn (HDN). The clinical importance of anti-K has resulted in the systematic determination of the K and Cellano antigens in both donors and patients. The ID-Cards **Anti-K** and **Anti-k** can be used to determine the antigen status of donor blood prior to crossmatching, for confirmation of the antigen after antibody identification, or for paternal/fetal antigen typing in allo-immunized pregnancies.

DiaClon Anti-K

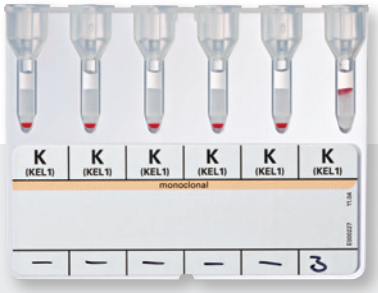

Ordering Information

Catalog #	Description
DiaClon Anti-K	
002121	**6 x K** (Id-n°: 50200) **72 tests**, 1 x 12

Cell line: MS-56

Anti-k

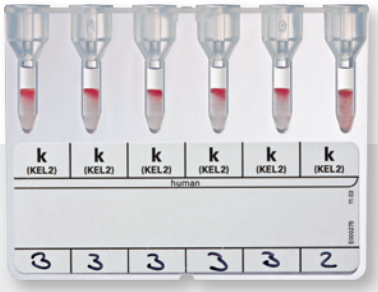

Ordering Information

Catalog #	Description
Anti-k	
007251	**6 x k** (Id-n°: 50260) human **72 tests**, 1 x 12

M (MNS1) and N (MNS2) antigenic determinants are carried on glycophorin A (GPA), one of the major sialic acid containing structure of the Red Blood Cell membrane.

According to Reid, M.E. [5], the phenotype frequencies of the MNS Blood Group System in the Caucasian population are as follows:

MM	28%
MN	50%
NN	22%

DiaClon Anti-M

Ordering Information

Catalog # Description

DiaClon Anti-M

007011 **6 x M** (Id-n°: 50212) **72 tests**, 1 x 12

Cell lines: 9211 9D5 1G10

DiaClon Anti-N

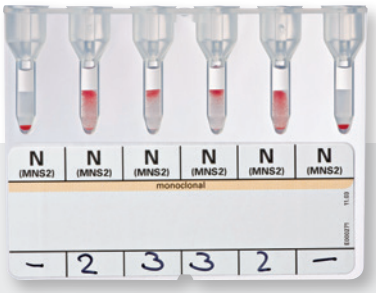

Ordering Information

Catalog # Description

DiaClon Anti-N

007111 **6 x N** (Id-n°: 50221) **72 tests**, 1 x 12

Cell lines: 1422 C7+MN879

DiaClon Anti-M/N

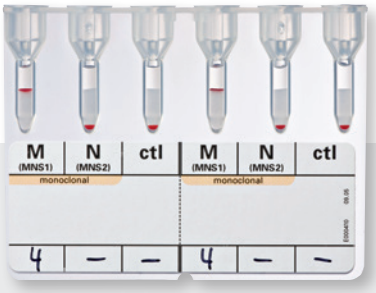

Ordering Information

Catalog # Description

DiaClon Anti-M/N

006011 **M, N, ctl/M, N, ctl** (Id-n°: 51210) **24 tests**, 1 x 12

Cell lines: **M:** 9211 9D5 1G10, **N:** 1422 C7+MN879

According to Reid, M.E. [5], the phenotype frequencies in the Caucasian population are:

Phenotype	Antigens	Frequency
P_1	$PP1P^k$	79%
P_2	PP^k	21%
p	-	very rare
P_1^k	$P1P^k$	very rare
P_2^k	P^k	very rare

DiaClon Anti-P_1

Ordering Information

Catalog #	Description
DiaClon Anti-P_1	
007212	**6 x P_1** (Id-n°: 51180) **72 tests**, 1 x 12

Cell line: 650

Lewis antigens are absent or only poorly expressed on Red Blood Cells from newborns. According to Reid, M.E. [5], the Lewis phenotype frequency in the Caucasian population is as follows:

Le(a-b+)	72%
Le(a+b-)	22%
Le(a-b-)	6%
Le(a+b+)	very rare*

** more common in East Asia, South East Asia, the Pacific region and Australia*

DiaClon Anti-Le^{a}

Ordering Information

Catalog # Description

DiaClon Anti-Le^{a}
007221 **6 x Le^{a}** (Id-n°: 50242) **72 tests**, 1 x 12

Cell lines: P3N20V3 + LM112/161

DiaClon Anti-Le^{b}

Ordering Information

Catalog # Description

DiaClon Anti-Le^{b}
007231 **6 x Le^{b}** (Id-n°: 50250) **72 tests**, 1 x 12

Cell lines: LM129/181 (LB1)

DiaClon Anti-Le^{a}/Le^{b}

Ordering Information

Catalog # Description

DiaClon Anti-Le^{a}/Le^{b}
006041 **Le^{a}, Le^{b}, ctl/Le^{a}, Le^{b}, ctl** (Id-n°: 51241) **24 tests**, 1 x 12

Cell lines: **Le^{a}:** P3N20V3 + LM112/161, **Le^{b}:** LM129/181 (LB1)

The antibodies of the Kidd Blood Group System are often associated with severe hemolytic transfusion reactions (HTRs), notably delayed reactions. The transfusion of compatible blood in the Kidd Blood Group System, where antibodies have previously been detected (or are suspected), is therefore important.

According to Reid, M.E. [5], the phenotype frequency of the antithetical Kidd antigens Jk^a and Jk^b in the Caucasian population is as follows:

Jk(a+b-)	26%
Jk(a+b+)	50%
Jk(a-b+)	24%
Jk(a-b-)	exceedingly rare

DiaClon Anti-Jk^a

Ordering Information

Catalog # Description

DiaClon Anti-Jk^a
007321 **6 x Jk^a** (Id-n°: 50270) **72 tests**, 1 x 12

Cell line: MS-15

DiaClon Anti-Jk^b

Ordering Information

Catalog # Description

DiaClon Anti-Jk^b
007331 **6 x Jk^b** (Id-n°: 50280) **72 tests**, 1 x 12

Cell line: MS-8

DiaClon Anti-Jk^a/Jk^b

Ordering Information

Catalog # Description

DiaClon Anti-Jk^a/Jk^b
006051 **Jk^a, Jk^b, ctl/Jk^a, Jk^b, ctl** (Id-n°: 51250) **24 tests**, 1 x 12

Cell lines: **Jk^a:** MS-15, **Jk^b:** MS-8

Kp^a (KEL3), Kp^b (KEL4) and Kp^c (KEL21) are part of the Kell (KEL) Blood Group System (ISBT, number 006). Kp^a is present in approximately 2% of the Caucasian population while Kp^b is a high frequency (public) antigen. The Kp^c antigen has an occurrence of less than 0.01% but up to 0.32% in Japanese.
Anti-Kp^a and anti-Kp^b are less common than anti-K but have similar serological characteristics and are considered to be clinically significant. They may occur after transfusion or by feto-maternal immunization.

According to Reid, M.E. [5], the phenotype frequency in the Caucasian population of the two most important antigens is as follows:

Kp(a+b-)	rare
Kp(a+b+)	± 2.3%
Kp(a-b+)	± 97.7%

Anti-Kp^a

Ordering Information

Catalog #	Description
Anti-Kp^a	
007301	**6 x Kp^a** (Id-n°: 50290) human **72 tests**, 1 x 12

Anti-Kp^b

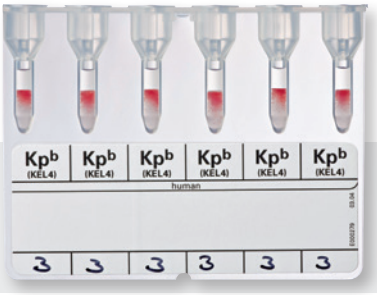

Ordering Information

Catalog #	Description
Anti-Kp^b	
007311	**6 x Kp^b** (Id-n°: 50300) human **72 tests**, 1 x 12

Anti-Kp^a/Kp^b

Ordering Information

Catalog #	Description
Anti-Kp^a/Kp^b	
006061	**Kp^a, Kp^b, ctl/Kp^a, Kp^b, ctl** (Id-n°: 51260) human **24 tests**, 1 x 12

Antibodies against antigens in the Lutheran Blood Group System are not often encountered.
The antigen-antibody reaction produces small and loose agglutinates in a characteristic mixed-field appearance.
The antigens are poorly developed at birth.
Allo anti-Lu^a has not been implicated in transfusion reactions and only rarely as causing mild hemolytic disease of the fetus and newborn (HDFN). Allo anti-Lu^b has been implicated in mild to moderate transfusion reactions and mild HDFN.

According to Reid, M.E. [5], the phenotype frequency of the Lutheran Blood Group System in most population is as follows:

Lu(a+b-)	0.2%
Lu(a+b+)	7.4%
Lu(a-b+)	92.4%
Lu(a-b-)	rare

Anti-Lu^a

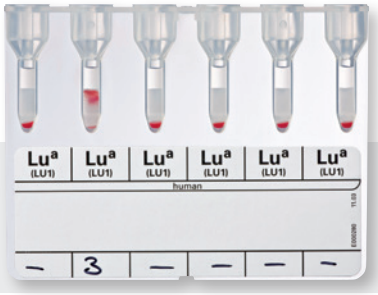

Ordering Information

Catalog #	Description
Anti-Lu^a	
007351	**6 x Lu^a** (Id-n°: 50310) human **72 tests**, 1 x 12

Anti-Lu^b

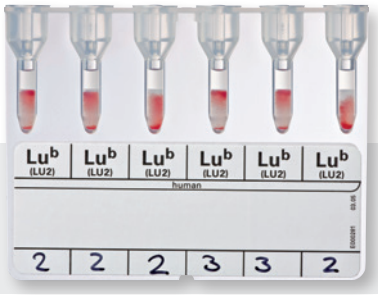

Ordering Information

Catalog #	Description
Anti-Lu^b	
007361	**6 x Lu^b** (Id-n°: 50320) human **72 tests**, 1 x 12

Anti-Lu^a/Lu^b

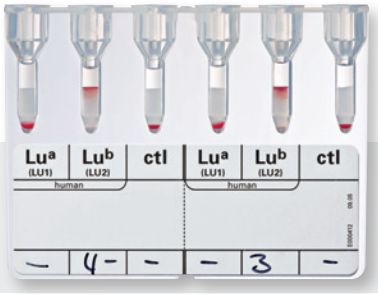

Ordering Information

Catalog #	Description
Anti-Lu^a/Lu^b	
006031	**Lu^a, Lu^b, ctl/Lu^a, Lu^b, ctl** (Id-n°: 51230) human **24 tests**, 1 x 12

The antigens S (MNS3) and s (MNS4) are carried on the human glycophrin B (GPB) molecule and are part of the MNS Blood Group System. Ss antibodies are not frequently encountered, however they have both been implicated in rare cases of severe hemolytic disease of the newborn and rare cases of mild to moderate hemolytic transfusion reactions, and are therefore clinically important.
Antigen typing of paternal or fetal/neonatal or donor blood may therefore also be appropriate, according to the clinical situation.

According to Daniels, G. [4], the phenotype frequency of the antithetical antigens S and s in the Caucasian population is as follows:

SS	11%
Ss	44%
ss	45%

Test of Antigen S
ID-Card S, Test Serum ID-Anti-S

Ordering Information

Catalog #	Description
ID-Card S, ID-Anti-S	
007130	**ID-Card S: 6 x S** (Id-n°: 50330) **72 tests**, 1 x 12
007132	**Test serum ID-Anti-S** (Id-n°: 09010) human **90 tests**, 1 x 5 ml

Test of Antigen s
ID-Card s, Test Serum ID-Anti-s

Ordering Information

Catalog #	Description
ID-Card s, ID-Anti-s	
007140	**ID-Card s: 6 x s** (Id-n°: 50340) **72 tests**, 1 x 12
007142	**Test serum ID-Anti-s** (Id-n°: 09110) human **90 tests**, 1 x 5 ml

Test of Antigen S and s
ID-Card S/s, Test Serum ID-Anti-S/s

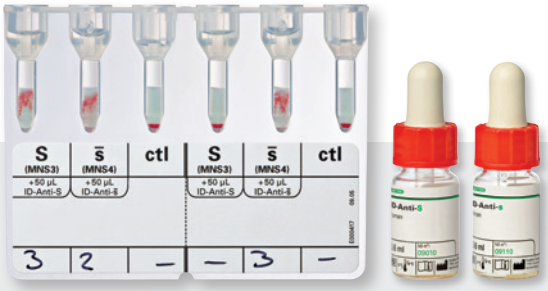

Ordering Information

Catalog #	Description
ID-Card S/s, ID-Anti-S/s	
006120	**ID-Card S/s: S, s, ctl/S, s, ctl** (Id-n°: 51280) **24 tests**, 1 x 12
007132	**Test serum ID-Anti-S** (Id-n°: 09010) human **90 tests**, 1 x 5 ml
007142	**Test serum ID-Anti-s** (Id-n°: 09110) human **90 tests**, 1 x 5 ml

Both Duffy antigens are fully developed at birth. Fy^a frequently causes immunization while Fy^b is rarely the cause of immunization. Anti-Fy^a and anti-Fy^b are practically always of immune origin.

They both cause hemolytic transfusion reactions and can, although not frequently, cause hemolytic disease of the newborn (HDN).

According to Reid, M.E. [5], the phenotype frequency of the Duffy Blood Group System is as follows:

	Caucasian	Blacks	Chinese	Japanese	Thai
Fy(a+b-)	17%	9%	90.80%	81.50%	69%
Fy(a-b+)	34%	22%	0.30%	0.90%	3%
Fy(a+b+)	49%	1%	8.90%	17.60%	28%
Fy(a-b-)	very rare	68%	0%	0%	0%

Test of Antigen Fy^a
ID-Card Fy^a, Test Serum ID-Anti-Fy^a

Ordering Information

Catalog #	Description
ID-Card Fy^a, ID-Anti-Fy^a	
007270	**ID-Card Fy^a: 6 x Fy^a** (Id-n°: 50350) **72 tests**, 1 x 12
007272	**Test serum ID-Anti-Fy^a** (Id-n°: 09210) human **90 tests**, 1 x 5 ml

Test of Antigen Fy^b
ID-Card Fy^b, Test Serum ID-Anti-Fy^b

Ordering Information

Catalog #	Description
ID-Card Fy^b, ID-Anti-Fy^b	
007280	**ID-Card Fy^b: 6 x Fy^b** (Id-n°: 50360) **72 tests**, 1 x 12
007282	**Test serum ID-Anti-Fy^b** (Id-n°: 09310) human **90 tests**, 1 x 5 ml

Test of Antigen Fy^a and Fy^b, ID-Card Fy^a/Fy^b, Test Serum ID-Anti-Fy^a/Fy^b

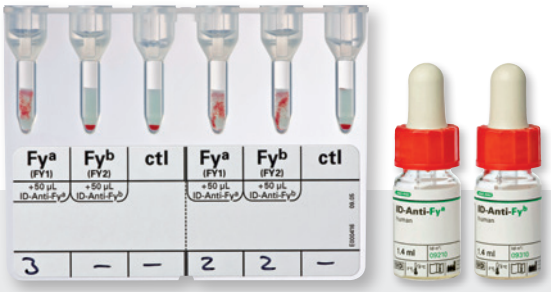

Ordering Information

Catalog #	Description
ID-Card Fy^a/Fy^b, ID-Anti-Fy^a/Fy^b	
006110	**ID-Card Fy^a/Fy^b: Fy^a, Fy^b, ctl/Fy^a, Fy^b, ctl** (Id-n°: 51270) **24 tests**, 1 x 12
007272	**Test serum ID-Anti-Fy^a** (Id-n°: 09210) human **90 tests**, 1 x 5 ml
007282	**Test serum ID-Anti-Fy^b** (Id-n°: 09310) human **90 tests**, 1 x 5 ml

Di^a is a low prevalence antigen, antithetical to Di^b and both antigens belong to the Diego Blood Group System.

Anti-Di^a may be responsible for severe transfusion reactions and hemolytic disease of the fetus and newborn (HDFN).

According to Reid, M.E. [5], the Di^a antigen occurrence is from 0.01% in most population and can be up to 54% in South American Indians.

Bio-Rad ID-Anti-Di^a test sera for use by Indirect Antiglobulin Test (IAT) with the ID-Card **LISS/Coombs** is from human sera containing incomplete antibodies.

ID-Anti-Di^a

Ordering Information

Catalog #	Description
ID-Anti-Di^a	
007420	**ID-Anti-Di^a: vial** (Id-n°: 09080) **10 tests**, 1 x 0.5 ml

According to availability

LISS/Coombs

The most important function of the polyspecific AHG reagent is to detect the presence of IgG. The importance of anti-complement in the AHG reagent is debatable since antibodies detectable only by their ability to bind complement are rather rare.

However, anti-C3d activity is important for the DAT in the investigation of autoimmune hemolytic anemia (AIHA).

A positive DAT generally indicates that the Red Blood Cells are coated *in vivo* with immunoglobulin and/or complement.

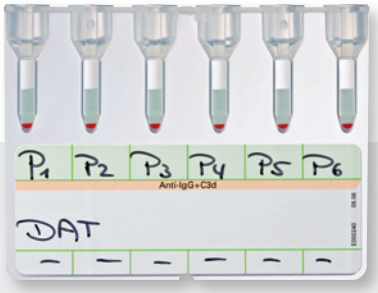

Ordering Information

Catalog #	Description
LISS/Coombs	
004014	**6 x AHG (Anti-IgG + C3d)** (Id-n°: 50531) rabbit **288 tests**, 4 x 12
004017	**6 x AHG (Anti-IgG + C3d)** (Id-n°: 50531) rabbit **1,728 tests**, 24 x 12
004016	**6 x AHG (Anti-IgG + C3d)** (Id-n°: 50531) rabbit **4,320 tests**, 60 x 12
004015	**6 x AHG (Anti-IgG + C3d)** (Id-n°: 50531) rabbit **8,064 tests**, 112 x 12

C3d: cell line C139-9

Coombs Anti-IgG

Some users prefer to use anti-IgG AHG serum because there is no interference from complement components which may be non-specifically bound to the Red Blood Cell.

Ordering Information

Catalog #	Description
Coombs Anti-IgG	
004024	**6 x AHG (Anti-IgG)** (Id-n°: 50540) rabbit **288 tests**, 4 x 12
004027	**6 x AHG (Anti-IgG)** (Id-n°: 50540) rabbit **1,728 tests**, 24 x 12
004026	**6 x AHG (Anti-IgG)** (Id-n°: 50540) rabbit **4,320 tests**, 60 x 12
004025	**6 x AHG (Anti-IgG)** (Id-n°: 50540) rabbit **8,064 tests**, 112 x 12

A positive Direct Antiglobulin Test (DAT) with polyspecific anti-human globulin (AHG) generally indicates that the Red Blood Cells are coated *in vivo* with immunoglobulin and/or complement.

To differentiate the reaction, monospecific AHG reagents are used, such as anti-IgG, -IgA, -IgM, -C3c and -C3d.

DC-Screening I

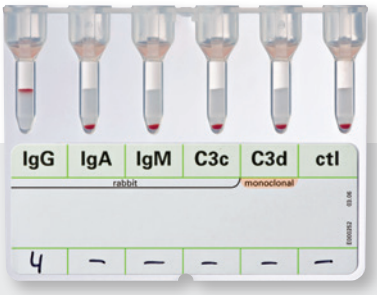

Ordering Information

Catalog #	Description
DC-Screening I	
004851	**IgG, IgA, IgM, C3c, C3d, ctl** (Id-n°: 50830) **12 profiles**, 1 x 12
004857	**IgG, IgA, IgM, C3c, C3d, ctl** (Id-n°: 50830) **288 profiles**, 24 x 12
004856	**IgG, IgA, IgM, C3c, C3d, ctl** (Id-n°: 50830) **720 profiles**, 60 x 12

IgG: rabbit, **IgA:** rabbit, **IgM:** rabbit, **C3c:** rabbit, **C3d:** cell line C139-9

DC-Screening II

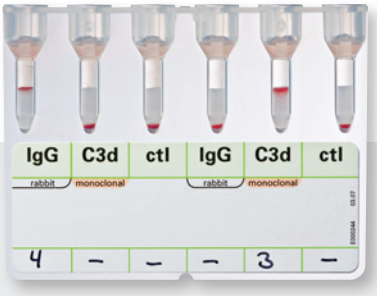

Ordering Information

Catalog #	Description
DC-Screening II	
004831	**IgG, C3d, ctl/IgG, C3d, ctl** (Id-n°: 50560) **24 profiles**, 1 x 12
004837	**IgG, C3d, ctl/IgG, C3d, ctl** (Id-n°: 50560) **576 profiles**, 24 x 12
004836	**IgG, C3d, ctl/IgG, C3d, ctl** (Id-n°: 50560) **1,440 profiles**, 60 x 12

IgG: rabbit, **C3d:** cell line C139-9

DAT IgG-Dilution

The numbers of IgG molecules per cell influence the accelerated Red Blood Cell destruction seen in Autoimmune Hemolytic Anemia (AIHA), Hemolytic Disease of the Newborn (HDN) and transfusion reactions.

The ID-Card **DAT IgG-Dilution** provides an indication of the clinical importance of the DAT positive result.

To further estimate the risk of hemolysis the differentiation of the IgG1 and IgG3 subclasses should be performed by using the ID-Card **DAT IgG1/IgG3**.

Ordering Information

Catalog #	Description
DAT IgG-Dilution	
004033	**1:10, 1:30, 1:100, 1:300, 1:1,000, ctl** (Id-n°: 50870) rabbit **12 profiles**, 1 x 12

DAT IgG1/IgG3

In the ID-Card **DAT IgG1/IgG3**, 2 dilutions of both anti-IgG1 and IgG3 are added to the gel, to allow the differentiation between low and high risk for hemolysis.

A positive reaction with the first dilution has a sensitivity of approximately 1,000 IgG1 and 125 IgG3 molecules/cells respectively.

A positive reaction with the second dilution indicates a high concentration of anti-IgG1 and/or IgG3 antibodies.

Ordering Information

Catalog #	Description
DAT IgG1/IgG3	
004043	**IgG subclasses** (Id-n°: 50890) **12 profiles**, 1 x 12

IgG1: cell line M345/795, **IgG3:** cell line M346/805

DiaScreen

The ID-Card **DiaScreen** consists of 4 microtubes containing polyspecific AHG for the IAT and 2 microtubes containing neutral gel for the two-stage enzyme technique.

Ordering Information

Catalog #	Description
DiaScreen	
004704	**4 x AHG tests/2 x enzyme tests** (Id-n°: 50571) **48 profiles**, 4 x 12
004707	**4 x AHG tests/2 x enzyme tests** (Id-n°: 50571) **288 profiles**, 24 x 12
004706	**4 x AHG tests/2 x enzyme tests** (Id-n°: 50571) **720 profiles**, 60 x 12
004705	**4 x AHG tests/2 x enzyme tests** (Id-n°: 50571) **1,344 profiles**, 112 x 12

AHG: rabbit, **C3d:** cell line C139-9

LISS/Coombs

Ordering Information

Catalog #	Description
LISS/Coombs	
004014	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **288 profiles**, 4 x 12
004017	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **1,728 profiles**, 24 x 12
004016	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **4,320 profiles**, 60 x 12
004015	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **8,064 profiles**, 112 x 12

C3d: cell line C139-9

Coombs Anti-IgG

Ordering Information

Catalog #	Description
Coombs Anti-IgG	
004024	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **288 profiles**, 4 x 12
004027	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **1,728 profiles**, 24 x 12
004026	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **4,320 profiles**, 60 x 12
004025	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **8,064 profiles**, 112 x 12

NaCl, Enzyme Test and Cold Agglutinins

The ID-Card **NaCl, Enzyme Test and Cold Agglutinins** is suitable for antibody screening and identification procedures, compatibility testing and reverse grouping.

It is not considered necessary to include the room temperature saline test in routine antibody screening procedures, but the saline test at 4°C can be used to detect cold agglutinins.

Ordering Information

Catalog #	Description
NaCl, Enzyme Test and Cold Agglutinins	
005014	**6 x tests** (Id-n°: 50520) **288 profiles**, 4 x 12
005017	**6 x tests** (Id-n°: 50520) **1,728 profiles**, 24 x 12
005016	**6 x tests** (Id-n°: 50520) **4,320 profiles**, 60 x 12
005015	**6 x tests** (Id-n°: 50520) **8,064 profiles**, 112 x 12

LISS/Coombs

Ordering Information

Catalog #	Description
LISS/Coombs	
004014	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **288 profiles**, 4 x 12
004017	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **1,728 profiles**, 24 x 12
004016	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **4,320 profiles**, 60 x 12
004015	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **8,064 profiles**, 112 x 12

C3d: cell line C139-9

Coombs Anti-IgG

Ordering Information

Catalog #	Description
Coombs Anti-IgG	
004024	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **288 profiles**, 4 x 12
004027	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **1,728 profiles**, 24 x 12
004026	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **4,320 profiles**, 60 x 12
004025	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **8,064 profiles**, 112 x 12

NaCl, Enzyme Test and Cold Agglutinins

The ID-Card **NaCl, Enzyme Test and Cold Agglutinins** is suitable for antibody screening and identification procedures, compatibility testing and reverse grouping.

It is not considered necessary to include the room temperature saline test in routine antibody screening procedures, but the saline test at 4°C can be used to detect cold agglutinins.

Ordering Information

Catalog #	Description
NaCl, Enzyme Test and Cold Agglutinins	
005014	**6 x tests** (Id-n°: 50520) **288 profiles**, 4 x 12
005017	**6 x tests** (Id-n°: 50520) **1,728 profiles**, 24 x 12
005016	**6 x tests** (Id-n°: 50520) **4,320 profiles**, 60 x 12
005015	**6 x tests** (Id-n°: 50520) **8,064 profiles**, 112 x 12

The methods used in compatibility tests should include those that will demonstrate ABO and RhD incompatibility and detect clinically significant unexpected antibodies.

The ID-Card **DiaClon Complete Crossmatch** is configured to meet the above requirements in one easy step:

- ABD-confirmation of both donor and/or recipient
- Major crossmatch test by the Indirect Antiglobulin Test (IAT)
- Major enzyme crossmatch test
- Autocontrol (IAT test)

DiaClon Complete Crossmatch

Ordering Information

Catalog #	Description
DiaClon Complete Crossmatch	
004614	**A, B, DVI-/Enz./2 x AHG** (Id-n°: 50601) **48 profiles**, 4 x 12
004617	**A, B, DVI-/Enz./2 x AHG** (Id-n°: 50601) **288 profiles**, 24 x 12
004616	**A, B, DVI-/Enz./2 x AHG** (Id-n°: 50601) **720 profiles**, 60 x 12
004615	**A, B, DVI-/Enz./2 x AHG** (Id-n°: 50601) **1,344 profiles**, 112 x 12

Cell lines: **A:** LM297/628 (LA-2), **B:** LM306/686 (LB-2), **D:** LHM59/20 (LDM3), 175-2, **AHG:** rabbit, **C3d:** cell line C139-9

LISS/Coombs

Ordering Information

Catalog #	Description
LISS/Coombs	
004014	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **288 profiles**, 4 x 12
004017	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **1,728 profiles**, 24 x 12
004016	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **4,320 profiles**, 60 x 12
004015	**6 x AHG (Anti-IgG + C3d) tests** (Id-n°: 50531) rabbit **8,064 profiles**, 112 x 12

C3d: cell line C139-9

Coombs Anti-IgG

Ordering Information

Catalog #	Description
Coombs Anti-IgG	
004024	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **288 profiles**, 4 x 12
004027	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **1,728 profiles**, 24 x 12
004026	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **4,320 profiles**, 60 x 12
004025	**6 x AHG (Anti-IgG) tests** (Id-n°: 50540) rabbit **8,064 profiles**, 112 x 12

NaCl, Enzyme Test and Cold Agglutinins

Ordering Information

Catalog #	Description
NaCl, Enzyme Test and Cold Agglutinins	
005014	**6 x tests** (Id-n°: 50520) **288 profiles**, 4 x 12
005017	**6 x tests** (Id-n°: 50520) **1,728 profiles**, 24 x 12
005016	**6 x tests** (Id-n°: 50520) **4,320 profiles**, 60 x 12
005015	**6 x tests** (Id-n°: 50520) **8,064 profiles**, 112 x 12

To ensure that appropriate therapeutic measures are instigated, DVI patients' Red Blood Cells should be assigned Rh negative status. Conversely, donor blood should be tested with anti-D that does detect DVI and assigned Rh positive status, to avoid the unit being transfused to an RhD negative or partial D patient.

DiaClon ABD-Confirmation for Patients

The ABD confirmation ID-Card can be used for the ABO/D blood group control of patients.

Ordering Information

Catalog #	Description
DiaClon ABD-Confirmation for Patients	
001254	**A, B, DVI-/A, B, DVI-** (Id-n°: 50053) **96 profiles**, 4 x 12
001257	**A, B, DVI-/A, B, DVI-** (Id-n°: 50053) **576 profiles**, 24 x 12
001256	**A, B, DVI-/A, B, DVI-** (Id-n°: 50053) **1,440 profiles**, 60 x 12
001255	**A, B, DVI-/A, B, DVI-** (Id-n°: 50053) **2,688 profiles**, 112 x 12

Cell lines: **A:** LM297/628 (LA-2), **B:** LM306/686 (LB-2), **D:** TH28, RUM-1, LDM1

DiaClon ABD-Confirmation for Donors

The ABD confirmation ID-Card can be used for the ABO/D blood group control of donors.

Ordering Information

Catalog #	Description
DiaClon ABD-Confirmation for Donors	
001134	**A, B, DVI+/A, B, DVI+** (Id-n°: 51051) **96 profiles**, 4 x 12
001133	**A, B, DVI+/A, B, DVI+** (Id-n°: 51051) **576 profiles**, 24 x 12
001136	**A, B, DVI+/A, B, DVI+** (Id-n°: 51051) **1,440 profiles**, 60 x 12
001135	**A, B, DVI+/A, B, DVI+** (Id-n°: 51051) **2,688 profiles**, 112 x 12

Cell lines: **A:** LM297/628 (LA-2), **B:** LM306/686 (LB-2), **D:** ESD-1M, 175-2

ID-Diluent 1

ID-Diluent 1 is a modified bromelin solution in which the enzyme activity is stabilised for a long period, specially prepared for the ID-System. **ID-Diluent 1** is used for preparing suspensions of Red Blood Cells for blood blood grouping, antigen typing and as an additive for enzyme tests with untreated Red Blood Cells for antibody detection and crossmatching.

Ordering Information

Catalog #	Description
ID-Diluent 1	
009160	**Modified Bromelin solution for Red Blood Cell suspensions and enzyme tests** (Id-n°: 05751), 2 x 100 ml
ID-Diluent 1 rack for IH-Analyzers	
009190	**Modified Bromelin solution for Red Blood Cell suspensions and enzyme tests** (Id-n°: 05751), 10 racks with 60 x 700 µl

ID-Diluent 2

ID-Diluent 2 is a modified low ionic strength solution made for the ID-System, for preparing 5% Red Blood Cell suspensions for blood grouping as well as 0.8% Red Blood Cell suspensions for crossmatching, autocontrol, direct anti-human globulin test, blood grouping of newborns, antigen typing and test cells prepared in the laboratory.

Ordering Information

Catalog #	Description
ID-Diluent 2	
009260	**Modified LISS for Red Blood Cell suspensions** (Id-n°: 05761), 2 x 100 ml
009280	**Modified LISS for Red Blood Cell suspensions** (Id-n°: 05761), 1 x 500 ml
ID-Diluent 2 rack for IH-Analyzers	
009290	**Modified LISS for Red Blood Cell suspensions** (Id-n°: 05761), 10 racks with 60 x 700 µl

ID-CellStab

ID-CellStab is a specially formulated glycine buffered saline which stabilizes Red Blood Cells at 0.8% suspension for use in the ID-System for up to 4 weeks after preparation.

Ordering Information

Catalog #	Description
ID-CellStab	
005650	**Stabilisation solution for Red Blood Cells** (Id-n°: 05740), 1 x 500 ml
005660	**Stabilisation solution for Red Blood Cells** (Id-n°: 05740), 2 x 100 ml

ID-CellWash-P

When required, Red Blood Cells can be papainized by the blood group laboratory, using **ID-Papain**, a standardized liquid papain solution. After treatment of the Red Blood Cells with papain, the cells must be washed with the specially prepared **ID-CellWash-P**.

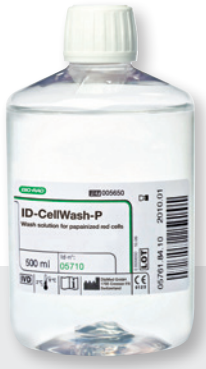

Ordering Information

Catalog #	Description
ID-CellWash-P	
005550	**Wash solution for papainized Red Blood Cells** (Id-n°: 05710), 1 x 500 ml

ID-Papain

ID-Papain is a standardized liquid papain solution and may be used for pre-treating Red Blood Cells by laboratories that prepare their own Red Blood Cell reagents, or may be used as an enzyme additive reagent in a one stage technique.

Ordering Information

Catalog #	Description
ID-Papain	
005510	**Papain solution for papainizing Red Blood Cells** (Id-n°: 06311), 1 x 10 ml

Stability 7 weeks, shipment on standing order, every 4 weeks

ID-Titration Solution

ID-Titration Solution is a dilution medium intended to be used for the titre determination of antibodies in patient and/or donor samples with the ID-System.

Combined with **ID-Titration Rack**, **ID-Titration Solution** can be used with IH-500 which leads to a higher accuracy in the dilution procedure and a better reliability of the overall titration process.

ID-Titration Solution is also suitable for manual use with the ID-System.

Ordering Information

Catalog #	Description
ID-Titration Solution	
009360	**Standardized medium for titration** (Id-n°: 05780), 10 x 10 ml
ID-Titration Rack	
009390	**Empty racks for the use on IH-500** (Id-n°: 05770), 10 racks of 60 wells

DiaCidel

Ordering Information

Catalog #	Description
DiaCidel	
108230	**For acid elution of serological antibodies** (Id-n°: 45630), 10 tests

Isoagglutinins (natural occurring antibodies, anti-A, anti-B, anti-AB) are cold reactive antibodies which react best at 4°C. However, they are also reactive at room temperature and may react at 37°C. They involve a mixture of IgM and IgG. The largest proportion, however, belongs to the IgM class.

ID-DiaCell ABO

All test cell reagents are of human origin, in a buffered suspension medium at 0.8% (± 0.1%).

Ordering Information

Catalog #	Description
ID-DiaCell ABO	
003619	**Set of 4 vials A_1, A_2, B, O** (Id-n°: 45022) **200 tests**, 4 x 10 ml
003615	**Set of 3 vials A_1, B, O** (Id-n°: 45352) **200 tests**, 3 x 10 ml
003624	**Set of 2 vials A_1, B** (Id-n°: 45092) **200 tests**, 2 x 10 ml
003621	**Single vial: A_2** (Id-n°: 06022) **200 tests**, 1 x 10 ml
003623	**Single vial: O** (Id-n°: 06042) **200 tests**, 1 x 10 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaScreen I-VI/Antigen Table (example)

	Rh-hr	Donor		Rh						Kell						Duffy		Kidd		Lewis		P	MNS				Luth.		Xg	
				D	C	E	c	e	C^w	K	k	Kp^a	Kp^b	Js^a	Js^b	Fy^a	Fy^b	Jk^a	Jk^b	Le^a	Le^b	P_1	M	N	S	s	Lu^a	Lu^b	Xg^a	F/M
I	$C^wCD.ee$	$R_1^wR_1$	675479	+	+	0	0	+	+	0	+	0	+	0	+	0	+	+	+	0	0	0	+	+	0	+	0	+	+	F
II	ccD.EE	R_2R_2	001251	+	0	+	+	0	0	0	+	0	+	0	+	+	+	+	0	+	0	+	0	+	+	+	+	+	+	M
III	ccddee	rr	060556	0	0	0	+	+	0	+	+	0	+	0	+	0	+	0	+	0	+	+	+	+	+	0	0	+	+	M
IV	CCD.ee	R_1R_1	887567	+	+	0	0	+	0	0	+	+	+	0	+	+	0	+	+	0	+	+	+	0	0	+	0	+	0	M
V	$C^wCD.ee$	$R_1^wR_1$	928899	+	+	0	0	+	+	+	+	0	+	0	+	0	+	0	+	+	0	+	+	+	+	+	0	+	+	F
VI	ccD.EE	R_2R_2	158648	+	0	+	+	0	0	0	+	0	+	0	+	+	+	+	0	0	+	+	+	0	+	+	0	+	+	M

Antigen tables are available electronically on ih-area.bio-rad.com and a printed version is provided with the products.

Fixed Rh Pattern I-III: $R_1^wR_1/R_2R_2/rr$

Four blood group O Red Blood Cells: Cell I: $R_1^wR_1$ (CCDee), C^w+ Cell II: R_2R_2 (ccDEE) Cell III: rr (ccee) Cell IV: (flexible Rh)	Enabling you to detect Rh-antibodies showing dosage
One cell K+	Enabling you to detect anti-K, a frequent antibody, alone or in combination
At least one cell double dose Fy^a, Fy^b, Jk^a, Jk^b, M, S and s	Enabling you to detect antibodies often showing dosage
All cells tested serologically for HLA-related antigens	Minimises nuisance caused by insignificant reactivity
Kp^a, C^w and Lu^a positive	Additional security and convenience
At least one cell positive for Le^a, Le^b, P_1 and N	

Fixed Rh Pattern V-VI: $R_1^wR_1$, R_2R_2

One cell is homozygous Jk(a+b-)	Enabling detection of anti-Jk^a showing dosage
One cell is Le(a+b-), the other Le(a-b+)	Additional security and convenience
One cell is C^w positive	Additional security and convenience

ID-DiaScreen

Expanded six-cell screening

- All the features of 3-cell screening
- PLUS two papain-treated cells
- PLUS one cell Kp(a+)
- PLUS one cell Lu(a+)

Ordering Information

Catalog #	Description
ID-DiaScreen	
004316	**Set of 6 vials for IAT and enzyme test I, II, III, IV, V, VI**
	$R_1^wR_1$, R_2R_2, rr, flexible Rh/$R_1^wR_1$, R_2R_2 papainized (Id-n°: 45070) **200 tests**, 6 x 10 ml
004311	**Set of 4 vials for IAT, I, II, III, IV**
	$R_1^wR_1$, R_2R_2, rr, flexible Rh (Id-n°: 45200) **200 tests**, 4 x 10 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaScreen Prophylax

The **ID-DiaScreen Prophylax**, though primarily for screening maternal samples after anti-D prophylaxis, is also very useful in immune anti-D investigations to aid detection/identification of further atypical alloantibodies.

To use with ID-Cards **LISS/Coombs** or **Anti-IgG**.

Screening maternal samples after anti-D prophylaxis

- One RhD positive and five RhD negative cells
- Double dose for Fy^a, Fy^b, Jk^a, Jk^b, M, S and s
- At least one cell positive for K, Le^a, Le^b, P_1 and N
- Tested by serology for HLA Class I antigens

Ordering Information

Catalog #	Description
ID-DiaScreen Prophylax	
004330	**Set of 6 vials for IAT R_1R_2, r'r, r''r, rr, rr, rr** (Id-n°: 45660) **100 tests**, 6 x 5 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaCell I-II-III/Antigen Table (example)

	Rh-hr	Donor		Rh						Kell						Duffy		Kidd		Lewis		P	MNS				Luth.		Xg	
				D	C	E	c	e	C^w	K	k	Kp^a	Kp^b	Js^a	Js^b	Fy^a	Fy^b	Jk^a	Jk^b	Le^a	Le^b	P_1	M	N	S	s	Lu^a	Lu^b	Xg^a	F/M
I	$C^wCD.ee$	$R_1^wR_1$	754456	+	+	0	0	+	+	0	+	0	+	0	+	+	+	0	+	+	0	+	+	0	+	0	0	+	0	M
II	ccD.EE	R_2R_2	047144	+	0	+	+	0	0	0	+	+	+	0	+	+	0	+	+	0	+	0	+	+	+	+	0	+	+	M
III	ccddee	rr	101469	0	0	0	+	+	0	+	+	0	+	0	+	0	+	+	0	0	+	+	0	+	0	+	+	+	+	F

Antigen tables are available electronically on ih-area.bio-rad.com and a printed version is provided with the products.

Fixed Rh Pattern I-III: $R_1^wR_1/R_2R_2/rr$

Three group O, RhD positive cells: CCDee (R_1R_1) and ccDEE (R_2R_2) and one RhD negative cell: cc.ee (rr)	Enabling you to detect Rh-antibodies showing dosage
One cell K+	Enabling you to detect anti-K, alone or in combination
At least one cell double dose Fy^a, Fy^b, Jk^a, Jk^b, M, S and s	Enabling you to detect antibodies often showing dosage
All cells tested serologically for HLA-related antigens	Minimises nuisance caused by insignificant reactivity
Kp^a and Lu^a positive if available	Additional security and convenience
At least one cell positive for Le^a, Le^b, P_1 and N	

Cells from the same three individual donors available also in papain treaded format as ID-DiaCell IP-IIP-IIIP
Increased sensitivity in the detection of antibodies in the Rh, Kidd and Lewis Blood Group Systems
Antibodies to enzyme-sensitive antigens will not be detected: Duffy, MNS and Xg Blood Group Systems

ID-DiaCell I-II-III

Three-cell screening for patients

- Two RhD positive cells (CCDee, C^w+, ccDEE) and one cell RhD negative (ccddee)
- Double dose for Fy^a, Fy^b, Jk^a, Jk^b, M, S and s
- At least one cell positive for K, Le^a, Le^b, P_1 and N
- Tested by serology for HLA Class I antigens

Ordering Information

Catalog #	Description
ID-DiaCell I-II-III	
004310	**Set of 3 vials for IAT and NaCl test $R_1^wR_1$, R_2R_2, rr** (Id-n°: 45184) **200 tests**, 3 x 10 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaCell IP-IIP-IIIP

Three-cell screening for patients (papainized)

Ordering Information

Catalog #	Description
ID-DiaCell IP-IIP-IIIP	
005310	**Set of 3 vials for enzyme test $R_1^wR_1$, R_2R_2, rr papainized** (Id-n°: 45194) **200 tests**, 3 x 10 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaCell I-II/Antigen Table (example)

	Rh-hr	Donor		Rh						Kell						Duffy		Kidd		Lewis		P	MNS				Luth.		Xg	
				D	C	E	c	e	C^w	K	k	Kp^a	Kp^b	Js^a	Js^b	Fy^a	Fy^b	Jk^a	Jk^b	Le^a	Le^b	P_1	M	N	S	s	Lu^a	Lu^b	Xg^a	F/M
I	CCD.ee	R_1R_1	950823	+	+	0	0	+	0	+	+	0	+	0	+	0	+	0	+	+	0	+	0	+	0	+	0	+	+	F
II	ccD.EE	R_2R_2	090901	+	0	+	+	0	0	0	+	0	+	0	+	+	0	+	0	0	+	+	+	0	+	0	+	+	+	F

Antigen tables are available electronically on ih-area.bio-rad.com and a printed version is provided with the products.

Fixed Rh Pattern I-II: R_1R_1, R_2R_2

Two group O, RhD positive cells: CCDee (R_1R_1) and ccDEE (R_2R_2)	Enabling you to detect Rh-antibodies showing dosage
One cell K+	Enabling you to detect anti-K, alone or in combination
One cell Fy(a+b-), one cell Jk(a+b-)	Enabling you to detect anti-Fy^a/anti-Jk^a showing dosage
At least one cell positive for Fy^b, Jk^b, Le^b, P_1, M, N, S and s	Enabling you to detect clinically significant antibodies
All cells tested serologically for HLA-related antigens	Minimises nuisance caused by insignificant reactivity

ID-DiaCell I-II

Two-cell screening for donors

- Two RhD positive cells (CCDee and ccDEE)
- Double dose for Fy^a and Jk^a
- At least one cell positive for K, Fy^b, Jk^b, Le^a, Le^b, P_1, M, N, S and s
- Tested by serology for HLA Class I antigens

Ordering Information

Catalog #	Description
ID-DiaCell I-II	
003613	**Set of 2 vials for IAT and NaCl test R_1R_1, R_2R_2** (Id-n°: 45151) **200 tests**, 2 x 10 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaCell I-II-III Asia (Mi^a+)

Three-cell screening for patients

- Two RhD positive cells (CCDee and ccDEE)
- Double dose for Fy^a and Jk^a
- A least one cell positive for K, Fy^b, Jk^b, Le^a, Le^b, P_1, M, N, S, s and Mi^a
- Tested by serology for HLA Class I antigens

Ordering Information

Catalog #	Description
ID-DiaCell I-II-III Asia	
003614	**Set of 3 vials for IAT and NaCl test R_1R_1, R_2R_2, Mi^a+** (Id-n°: 45330) **200 tests**, 3 x 10 ml

Stability 7 weeks, shipment on standing order every 4 weeks
According to availability

ID-Di^a (Diego) Positive

Ordering Information

Catalog #	Description
ID-Di^a (Diego) Positive	
004134	**Single vial** (Id-n°: 05980) **200 tests**, 1 x 10 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-I Negative Cell

Ordering Information

Catalog #	Description
ID-I Negative Cell	
004111	**Single vial** (Id-n°: 06291) **32 tests**, 1 x 1.6 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaCell Pool

Ordering Information

Catalog #	Description
ID-DiaCell Pool	
003630	**2 pooled cells for IAT test R_1R_1, R_2R_2** (Id-n°: 06070) **200 tests**, 1 x 10 ml
003631	**2 pooled cells for IAT test R_1R_1, R_2R_2** (Id-n°: 06070) **600 tests**, 3 x 10 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaPanel 1-11/Antigen Table (example)

	Rh-hr	Donor		Rh						Kell						Duffy		Kidd		Lewis		P	MNS				Luth.		Xg	
				D	C	E	c	e	C^w	K	k	Kp^a	Kp^b	Js^a	Js^b	Fy^a	Fy^b	Jk^a	Jk^b	Le^a	Le^b	P_1	M	N	S	s	Lu^a	Lu^b	Xg^a	F/M
1	$C^wCD.ee$	$R_1^wR_1$	677783	+	+	0	0	+	+	0	+	0	+	0	+	+	0	+	0	0	+	+	+	0	+	0	0	+	+	
2	CCD.ee	R_1R_1	113683	+	+	0	0	+	0	+	+	0	+	0	+	0	+	+	+	0	0	+	0	+	0	+	0	+	0	
3	ccD.EE	R_2R_2	422278	+	0	+	+	0	0	0	+	0	+	0	+	+	+	0	+	0	+	+	+	+	+	0	0	+	+	
4	Ccddee	r'r	293832	0	+	0	+	+	0	0	+	0	+	0	+	+	0	0	+	+	0	+	+	+	+	+	0	+	+	
5	ccddEe	r''r	307849	0	0	+	+	+	0	0	+	0	+	0	+	+	+	+	+	0	+	+	+	+	0	+	+	+	0	
6	ccddee	rr	308478	0	0	0	+	+	0	+	+	0	+	0	+	0	+	0	+	0	0	+	0	+	0	+	0	+	nt	
7	ccddee	rr	439656	0	0	0	+	+	0	0	+	0	+	0	+	0	+	+	0	+	0	+	+	0	+	+	0	+	+	
8	ccD.ee	Ror	032656	+	0	0	+	+	0	0	+	0	+	0	+	0	0	+	0	0	0	+	0	+	0	+	0	+	0	
9	ccddee	rr	341656	0	0	0	+	+	0	0	+	0	+	0	+	+	0	0	+	0	+	0	0	+	0	+	0	+	0	
10	ccddee	rr	454253	0	0	0	+	+	0	0	+	0	+	0	+	0	+	0	+	0	+	0	0	+	+	0	0	+	+	
11	ccddee	rr	169276	0	0	0	+	+	0	0	+	+	+	0	+	+	0	+	+	0	+	+	+	0	0	+	0	+	+	

Two K+ cells, one D neg and one c neg — D neg cells (cc.ee), positive for Lewis — D neg cells, double dose cells for Duffy, Kidd and MNS
A Fy(a-b-) cell — CCDee; K-; Fy(a+b-) CCDee; K+; Fy(a-b+) — Fixed Rh pattern

Combined papain-treated and untreated panel — Fixed Rh pattern

Antigen tables are available electronically on ih-area.bio-rad.com and a printed version is provided with the products.

Fixed Rh pattern 1-11: $R_1^wR_1/R_1R_1/R_2R_2$/r'r/r"r/rr/rr/Ror/rr/rr/rr

11 group O adult cells	Allows identification of most single antibodies and simple antibody mixtures
Fixed Rh pattern	Allows identification of most single antibodies and simple antibody mixtures in the Rh Blood Group System
Minimum 2, maximum 3 K+ cells; one CCDee, other(s) ccddee	Allows identification of anti-K, alone or underlying anti-c/anti-D
Minimum 2, preferably 3 cells double dose for Fy^a, Fy^b, Jk^a, Jk^b, M, N, S and s	Allows identification of specific antibodies, even when they show dosage, and will allow underlying antibodies to be ruled out
Minimum 2 cells negative for Le^a, Le^b and P_1	Allows identification of specific antibodies, and will allow underlying antibodies to be ruled out
On the ccddee cells, minimum 1 cell homozygous for Fy^a, Fy^b, Jk^a, Jk^b, M, N, S and s	Allows identification of specific antibodies underlying anti-D, anti-CD, anti-CDE, including those showing dosage
On the ccddee cells, minimum 1 cell positive for Le^a, Le^b and P_1	Allows identification of specific antibodies underlying anti-D, anti-CD and anti-CDE
Minimum 2, maximum 3 Le(a-b-) cells	Allows identification of anti-Le^a and Le^b, common in prenatal patients and in Black populations
When available, one of the CCDee cells will be K+; Fy(a-b+) and the other K-; Fy(a+b-)	Allows identification of anti-K and/or anti-Fy^a underlying anti-c
One cell is always Fy(a-b-)	Allows identification of antibodies underlying anti-Fy^a or anti-Fy^b or to identify unusual antibodies in the Duffy Blood Group System
Standard and papain-treated panels	Offers improved efficiency and time saving and allows identification of routine, weak and complex antibody problems

ID-DiaPanel

Test Cells for Antibody Identification

- Fixed Rh phenotype pattern
- Assured presence of cells possessing double-dose antigens throughout
- Five ccddee cells carefully selected to assure double-dose of significant blood group antigens
- Tested by serology for HLA Class I antigens

Ordering Information

Catalog #	Description
ID-DiaPanel	
004114	**Set of 11 vials for IAT and NaCl test** (Id-n°: 45161) **80 tests**, 11 x 4 ml

Stability 7 weeks, shipment on standing order every 4 weeks

ID-DiaPanel Plus 6

Selected cells for complex problems

- Two additional c-negative, and two additional e-negative cells, all double dose for the significant blood group antigens
- One of the e-negative cells is K+
- Alternating presence of a CCDEe/CcDEE cell
- Alternating presence of a cell lacking a high incidence or possessing a low incidence antigen
- Tested by serology for HLA Class I antigens

Ordering Information

Catalog #	Description
ID-DiaPanel Plus 6	
004414	**Set of 6 vials for IAT and NaCl test** (Id-n°: 45670) **80 tests**, 6 x 4 ml

Stability 12 weeks, shipment on standing order every 8 weeks

ID-DiaPanel-P

Test cells for antibody identification in two-step papain test

Ordering Information

Catalog #	Description
ID-DiaPanel-P	
004214	**Set of 11 vials for enzyme test, papainized** (Id-n°: 45171) **80 tests**, 11 x 4 ml

Stability 7 weeks, shipment on standing order every 4 weeks

IH-QC Modular System

Transfusion guidelines recommend regular evaluation of test materials, test methods, local working instructions, and automated equipment and instruments used.
The control sample should always have the same characteristics as a patient sample and therefore be treated identically.

These activities are intended to ensure accuracy and safety of the blood grouping serological results. The controls should be carried out at regular intervals. Please refer to local/national guidelines.

IH-QC 1

4 tubes containing 6 ml of a human Red Blood Cells suspension (Hct 15%).

Ordering Information

Catalog #	Description
IH-QC 1	
009321	**Set of 4 tubes** (Id-n°: 08710), 4 x 6 ml, 1 Set

Supplies on standing order, every 4 weeks

IH-QC 2

4 tubes containing 6 ml of a human Red Blood Cells suspension (Hct 15%).

Ordering Information

Catalog #	Description
IH-QC 2	
009322	**Set of 4 tubes** (Id-n°: 08720), 4 x 6 ml, 1 Set

Supplies on standing order, every 4 weeks

IH-QC 3

4 tubes containing 6 ml of a human Red Blood Cells suspension (Hct 15%).

Ordering Information

Catalog #	Description
IH-QC 3	
009323	**Set of 4 tubes** (Id-n°: 08730), 4 x 6 ml, 1 Set

Supplies on standing order, every 4 weeks

IH-QC 4

4 tubes containing 6 ml of a human Red Blood Cells suspension (Hct 15%).

Ordering Information

Catalog #	Description
IH-QC 4	
009324	**Set of 4 tubes** (Id-n°: 08740), 4 x 6 ml, 1 Set

Supplies on standing order, every 4 weeks

IH-QC 5

4 tubes containing 6 ml of a human Red Blood Cells suspension (Hct 15%).

Ordering Information

Catalog #	Description
IH-QC 5	
009325	**Set of 4 tubes** (Id-n°: 08750), 4 x 6 ml, 1 Set

Supplies on standing order, every 4 weeks

Intended Use

IH-QC 1, **IH-QC 2**, **IH-QC 3**, **IH-QC 4** and **IH-QC 5** are intended to control the ID-System manually and/or with instruments for the determination of the ABO system, Rh (RH) system, Kell (KEL) system, and/or further immunohematology tests as listed below.

ANALYSIS	IH-QC 1	IH-QC 2	IH-QC 3	IH-QC 4	IH-QC 5
ABO forward and/or reverse grouping	✔	✔	✔	✔	✔
RhD typing	✔	✔	✔	✔	✔
Rh/K phenotyping	✔	✔	✔	✔	✔
Antibody screening/identification, Indirect Antiglobulin Test (IAT)	✔	✔	✔	✔	✔
Antibody screening/identification, 2 stage papain technique	✔	✔	✔	✖	✔
Crossmatch, Indirect Antiglobulin Test (IAT)	✔	✔	✔	✔	✔
Direct Antiglobulin Test (DAT)	✔	✔	✔	✔	✔

IH-QC 6

1 tube containing 6 ml of a human Red Blood Cells suspension (Hct 10%).

Ordering Information

Catalog #	Description
IH-QC 6	
009326	**Single tube** (Id-n°: 08760), 1 x 6 ml

Supplies on standing order, every 4 weeks

IH-QC 7

1 tube containing 6 ml of a human Red Blood Cells suspension (Hct 10%).

Ordering Information

Catalog #	Description
IH-QC 7	
009327	**Single tube** (Id-n°: 08770), 1 x 6 ml

Supplies on standing order, every 4 weeks

IH-QC 8

1 tube containing 6 ml of a human Red Blood Cells suspension (Hct 10%).

Ordering Information

Catalog #	Description
IH-QC 8	
009328	**Single tube** (Id-n°: 08780), 1 x 6 ml

Supplies on standing order, every 4 weeks

Intended Use

IH-QC 6, **IH-QC 7** and **IH-QC 8** are intended to control the ID-System manually and/or with instruments for the immunohematology tests listed below.

ANALYSIS	IH-QC 6	IH-QC 7	IH-QC 8
Direct Antiglobulin Test (DAT)	✔	✔	✔
RhD typing: direct testing and IAT	✔	✖	✖

Reagent Characteristics

	ABO	RH	K	FY	Antibodies		DAT
IH-QC 1	A_1 [ABO:1,-2,3,4]	ddccee (rr), C^w- [RH:-1,-2,-3,4,5,-8]	K+ [KEL:1]	N/A	Anti-B [Anti-ABO2]	Anti-D 0.05 IU/ml [Anti-RH1]	Neg
IH-QC 2	B [ABO:-1,2,3]	DCcEe (R_1R_2), C^w- [RH:1,2,3,4,5,-8]	K- [KEL:-1]	Fy(a-) [FY:-1]	Anti-A [Anti-ABO1]	Anti-Fy^a [Anti-FY1]	Neg
IH-QC 3	AB [ABO:1,2,3]	DCCee (R_1R_1), C^w- [RH:1,2,-3,-4,5,-8]	K- [KEL:-1]	N/A	Anti-c [Anti-RH4]		Neg
IH-QC 4	O [ABO:-1,-2,-3]	DccEE (R_2R_2), C^w- [RH:1,-2,3,4,-5,-8]	K- [KEL:-1]	N/A	Anti-A and Anti-B [Anti-ABO1 and Anti-ABO2]	Anti-K [Anti-KEL1]	Neg
IH-QC 5	A_2 [ABO:1,-2,3,-4]	DCcee (R_1r), C^w- [RH:1,2,-3,4,5,-8]	K- [KEL:-1]	N/A	Anti-B* [Anti-ABO2]		Neg
IH-QC 6	N/A	Weak D [RH:W1]	N/A	N/A	N/A		Neg
IH-QC 7	N/A	N/A	N/A	N/A	N/A		Pos [IgG]
IH-QC 8	N/A	N/A	N/A	N/A	N/A		Pos [C3b (c/d)]

** No irregular antibodies added - negative antibody screening/identification*

N/A: Not Applicable

Anti-D Reference-Reagent has been developed to assist in the daily quality monitoring of routine antibody detection procedures.
A standardized dilution of the **Anti-D Reference-Reagent** should be used as a control to validate the sensitivity of routine test methods and reagents used.

It may also be used at appropriate dilutions for the proficiency testing of laboratory staff.

Bovine Albumin 6% is required as additional reagent for the dilution of the **Anti-D Reference-Reagent**.

Anti-D Reference Reagent

Monoclonal for controlling antibody detection procedures.

Ordering Information

Catalog #	Description
Anti-D Reference Reagent	
105500	**Anti-D Reference Reagent** (Id-n°: 13010), 6 x 0.5 ml

Cell lines: ESD 1 and LHM59/19

Albumin 6%

Ordering Information

Catalog #	Description
Albumin 6%	
105519	**Bovine Albumin 6%** (Id-n°: 13030), 1 x 10 ml
105520	**Bovine Albumin 6%** (Id-n°: 13030), 10 x 10 ml

Transfusion guidelines recommend regular checking of test materials, test methods, personnel, working procedures and automated equipment/instruments used. The control sample should always have the same characteristics as a patient/donor sample and therefore be treated identically.

These activities are intended to ensure the accuracy and safety of the blood group serological results.

ID-Internal Quality Control

ID-Internal Quality Control contains 5 vials of 4 ml human Red Blood Cell reagent from single donors as a 3-5% suspension in a buffered medium, and 3 vials with 3 ml serum of human origin.

Ordering Information

Catalog #	Description
ID-Internal Quality Control	
009925	**Set of 5 x 4 ml Red Blood Cells and 3 x 3 ml sera** (Id-n°: 45341) **80 tests**, 1 Set

Supplies on standing order, every 4 weeks

ANALYSIS	Sample 1	Sample 2	Sample 3	Sample 4	Sample 5
ABO forward grouping	✔	✔	✔	✔	✖
RhD typing	✔	✔	✔	✔	✖
Rh phenotyping	✖	✔	✔	✖	✖
K phenotyping	✖	✖	✔	✖	✖
Direct Antiglobulin Test (DAT)	✖	✖	✖	✖	✔

ANALYSIS	Serum 1	Serum 2	Serum 3
ABO reverse grouping	✔	✔	✔
Antibody screening/identification	✔	✔	✔

Reagent Characteristics

	ABO	RH	K	Antibodies		DAT
Sample 1	AB [ABO:1,2,3]	RhD positive	N/A	N/A	N/A	N/A
Sample 2	O [ABO:-1,-2,-3]	ddccee (rr) [RH:-1,-2,-3,4,5]	N/A	N/A	N/A	N/A
Sample 3	O [ABO:-1,-2,-3]	DCcEe (R_1R_2) [RH:1,2,3,4,5]	K+ [KEL:1]	N/A	N/A	N/A
Sample 4	O [ABO:-1,-2,-3]	Weak D	N/A	N/A	N/A	N/A
Sample 5	N/A	N/A	N/A	N/A	N/A	Pos
Serum 1	N/A	N/A	N/A	none	Anti-Fy^a* [Anti-FY1]	N/A
Serum 2	N/A	N/A	N/A	Anti-A and Anti-B [Anti-ABO1 and Anti-ABO2]	Anti-E* [Anti-RH4]	N/A
Serum 3	N/A	N/A	N/A	Anti-A and Anti-B [Anti-ABO1 and Anti-ABO2]	none	N/A

** 2 sera with irregular antibodies, which can change from lot to lot*
N/A: Not Applicable

Notes

Bio-Rad
Laboratories, Inc.

Clinical
Diagnostics Group

Contact LABEX, your Bio-Rad partner for more information:
Sweden +4642324000 Norway: +476679020 Denmark +4545661300
sales@labex.com www.labex.com

Bulletin H010111

© 2023 Bio-Rad Laboratories, Inc. 2023/03